

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\
Quantitation Report (QT Reviewed)


Data File : VV013351.D
Acq On : 25 Oct 2019 17:20
Operator : SY/MD
Sample : K5462-21
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G25

Manual Integrations
APPROVED

MMDadoda
10/28/2019 9:49:03 AM

Quant Time: Oct 26 01:49:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 26 00:57:59 2019
Response via : Initial Calibration

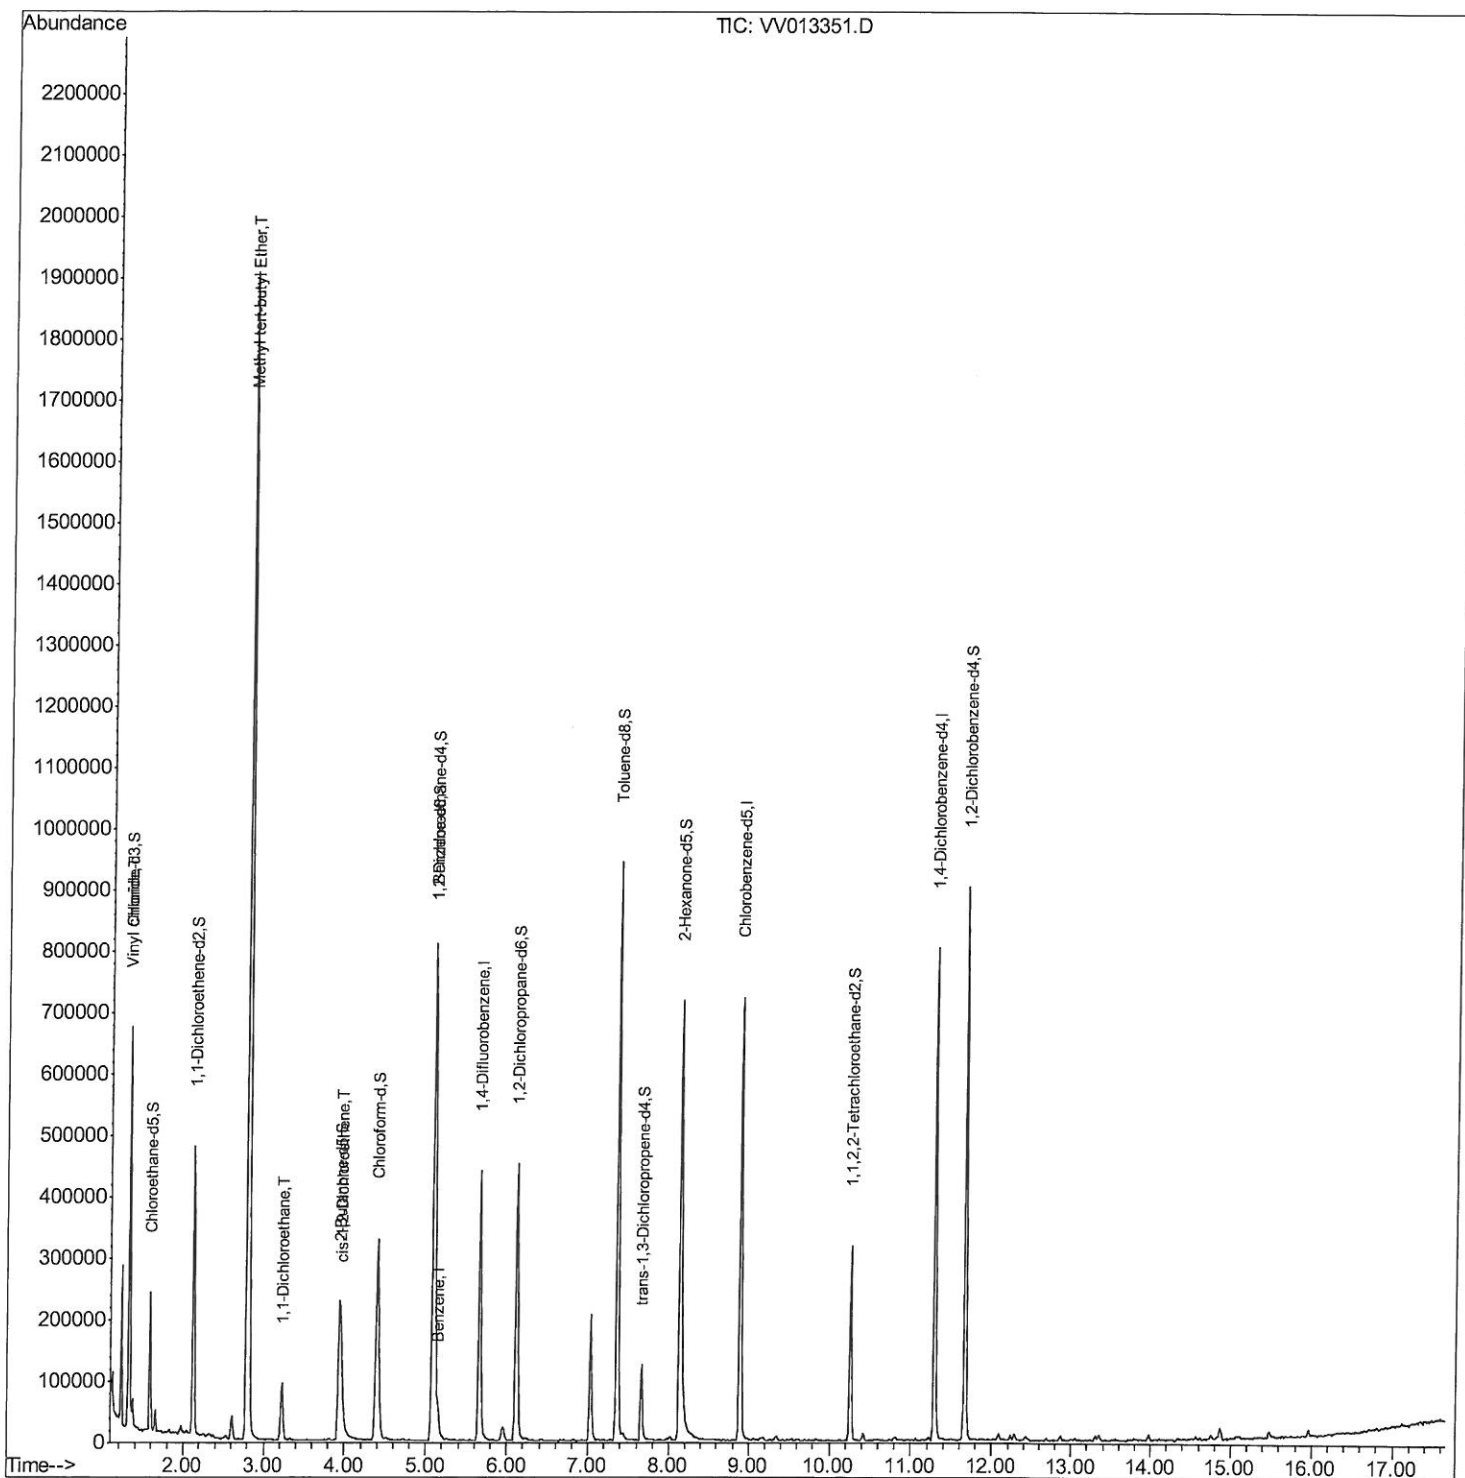

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\
Quantitation Report (Qedit)




Data File : VV013351.D
Acq On : 25 Oct 2019 17:20
Operator : SY/MD
Sample : K5462-21
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G25

Manual Integrations
APPROVED

MMDadoda
10/28/2019 9:49:03 AM

Quant Time: Oct 26 01:02:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 26 00:57:59 2019
Response via : Initial Calibration

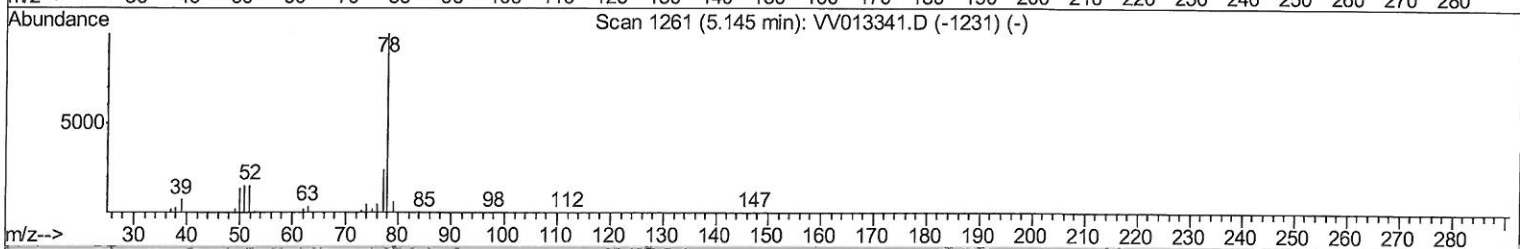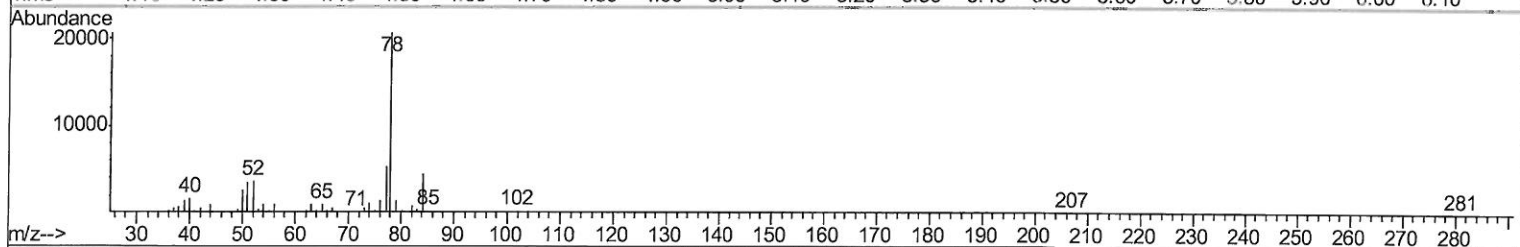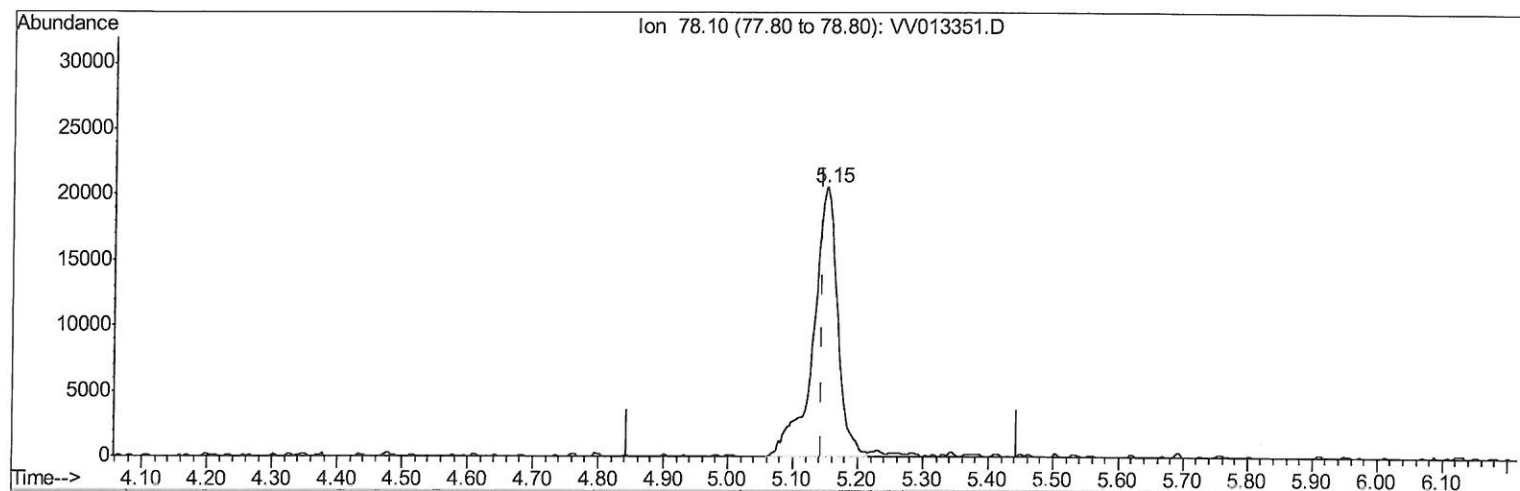

TIC: VV013351.D

(33) Benzene (T)

5.151min (+0.006) 0.33ug/L

response 53757

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\
Quantitation Report (Qedit)




Data File : VV013351.D
Acq On : 25 Oct 2019 17:20
Operator : SY/MD
Sample : K5462-21
Misc : 25.0ML/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G25

Manual Integrations
APPROVED

MMDadoda
10/28/2019 9:49:03 AM

Quant Time: Oct 26 01:02:14 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 26 00:57:59 2019
Response via : Initial Calibration

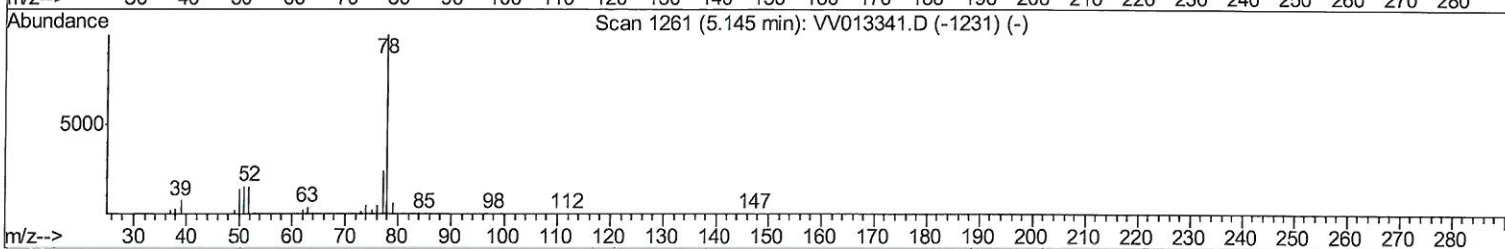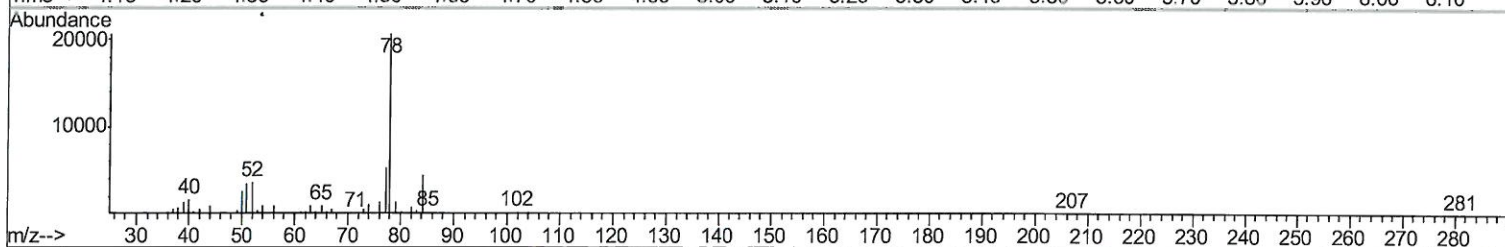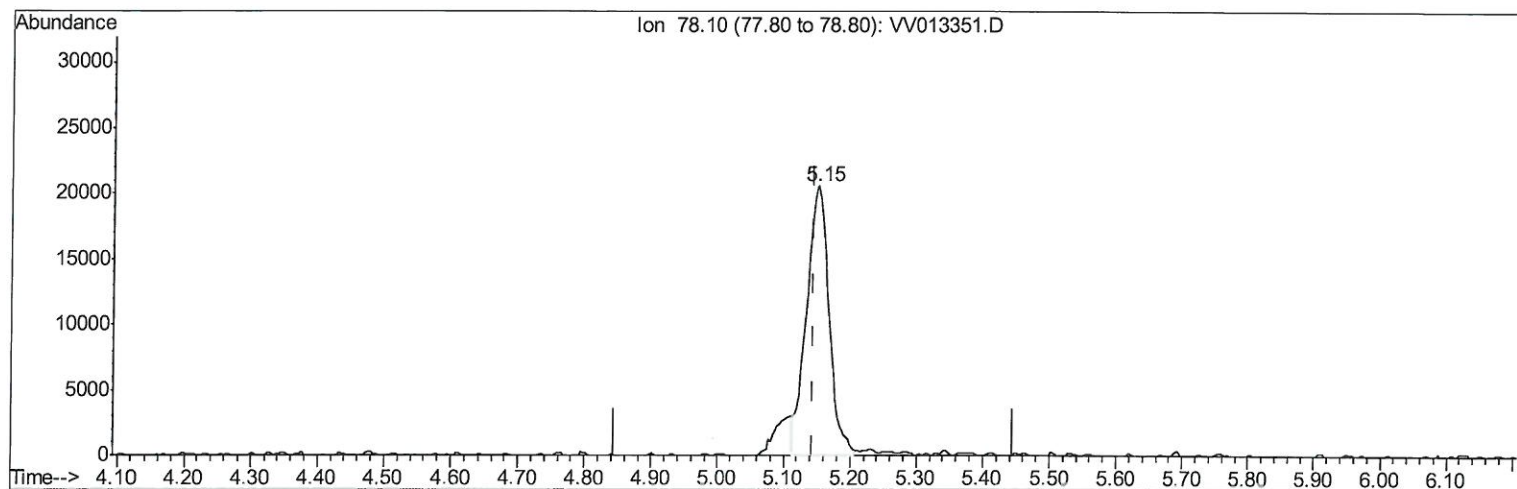

TIC: VV013351.D

(33) Benzene (T)

5.151min (+0.006) 0.30ug/L m

response 48021

Ion	Exp%	Act%
78.10	100	100
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00

MD
10/26/19

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102519\

Quantitation Report (QT Reviewed)

Data File : VV013351.D

Acq On : 25 Oct 2019 17:20

Operator : SY/MD

Sample : K5462-21

Misc : 25.0ML/MSVOA_V/WATER

ALS Vial : 12 Sample Multiplier: 1

Instrument :

MSVOA_V

ClientSampleId :

H0G25

Manual Integrations

APPROVED

MMDadoda

10/28/2019 9:49:03 AM

Quant Time: Oct 26 01:49:50 2019

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M

Quant Title : TRACE VOA SOM01.0

QLast Update : Sat Oct 26 00:57:59 2019

Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	394803	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	423570	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	230276	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	190229	6.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	130.80%#
7) Chloroethane-d5	1.58	69	144960	6.03	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	120.60%
11) 1,1-Dichloroethene-d2	2.13	63	231452	4.47	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	89.40%
20) 2-Butanone-d5	3.94	46	367684	65.78	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	131.56%#
24) Chloroform-d	4.40	84	337140	4.93	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	98.60%
26) 1,2-Dichloroethane-d4	5.08	65	168369	5.31	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	106.20%
32) Benzene-d6	5.10	84	766037	5.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	111.80%
36) 1,2-Dichloropropane-d6	6.12	67	222837	5.40	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	108.00%
41) Toluene-d8	7.36	98	638836	5.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.60%
43) trans-1,3-Dichloropropene-	7.66	79	74220	4.75	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.00%
46) 2-Hexanone-d5	8.13	63	228655	41.09	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	82.18%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	145923	4.90	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	264517	5.90	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	118.00%

Target Compounds

					Qvalue	
5) Vinyl chloride	1.32	62	98926	2.596	ug/L	96
17) Methyl tert-butyl Ether	2.80	73	1915105	26.640	ug/L	97
19) 1,1-Dichloroethane	3.23	63	94069	1.582	ug/L	98
22) cis-1,2-Dichloroethene	3.96	96	26770	0.683	ug/L #	89
33) Benzene	5.15	78	48021m	0.297	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

JMD
10/26/19