

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102519\
 Data File : VV013352.D
 Acq On : 25 Oct 2019 17:44
 Operator : SY/MD
 Sample : K5462-19
 Misc : 25.0ML/MSVOA V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0G17

Quant Time: Oct 26 01:58:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Oct 26 00:57:59 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	400469	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	433704	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	230163	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	186410	6.31	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	126.20%
7) Chloroethane-d5	1.58	69	143930	5.91	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	118.20%
11) 1,1-Dichloroethene-d2	2.13	63	226928	4.32	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	86.40%
20) 2-Butanone-d5	3.94	46	375569	66.24	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	132.48%#
24) Chloroform-d	4.40	84	348620	5.02	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.40%
26) 1,2-Dichloroethane-d4	5.08	65	166486	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	5.10	84	752606	5.36	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	107.20%
36) 1,2-Dichloropropane-d6	6.11	67	223076	5.28	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	105.60%
41) Toluene-d8	7.36	98	649453	4.99	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.80%
43) trans-1,3-Dichloropropene-	7.66	79	74833	4.68	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	93.60%
46) 2-Hexanone-d5	8.13	63	226306	39.72	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	79.44%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	143015	4.69	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	93.80%
64) 1,2-Dichlorobenzene-d4	11.67	152	260977	5.83	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.60%

Target Compounds


					Ovalue
5) Vinyl chloride	1.32	62	145062	3.753	ug/L 97
17) Methyl tert-butyl Ether	2.80	73	2533046	34.737	ug/L 97
18) trans-1,2-Dichloroethene	2.79	96	177588	4.784	ug/L 92
19) 1,1-Dichloroethane	3.23	63	73545	1.219	ug/L 98
22) cis-1,2-Dichloroethene	3.96	96	1675062	42.163	ug/L # 92
33) Benzene	5.14	78	34858	0.210	ug/L 100
34) Trichloroethene	5.96	95	747647	16.825	ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102519\
Data File : VV013352.D
Acq On : 25 Oct 2019 17:44
Operator : SY/MD
Sample : K5462-19
Misc : 25.0ML/MSVOA V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0G17

Quant Time: Oct 26 01:58:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Oct 26 00:57:59 2019
Response via : Initial Calibration

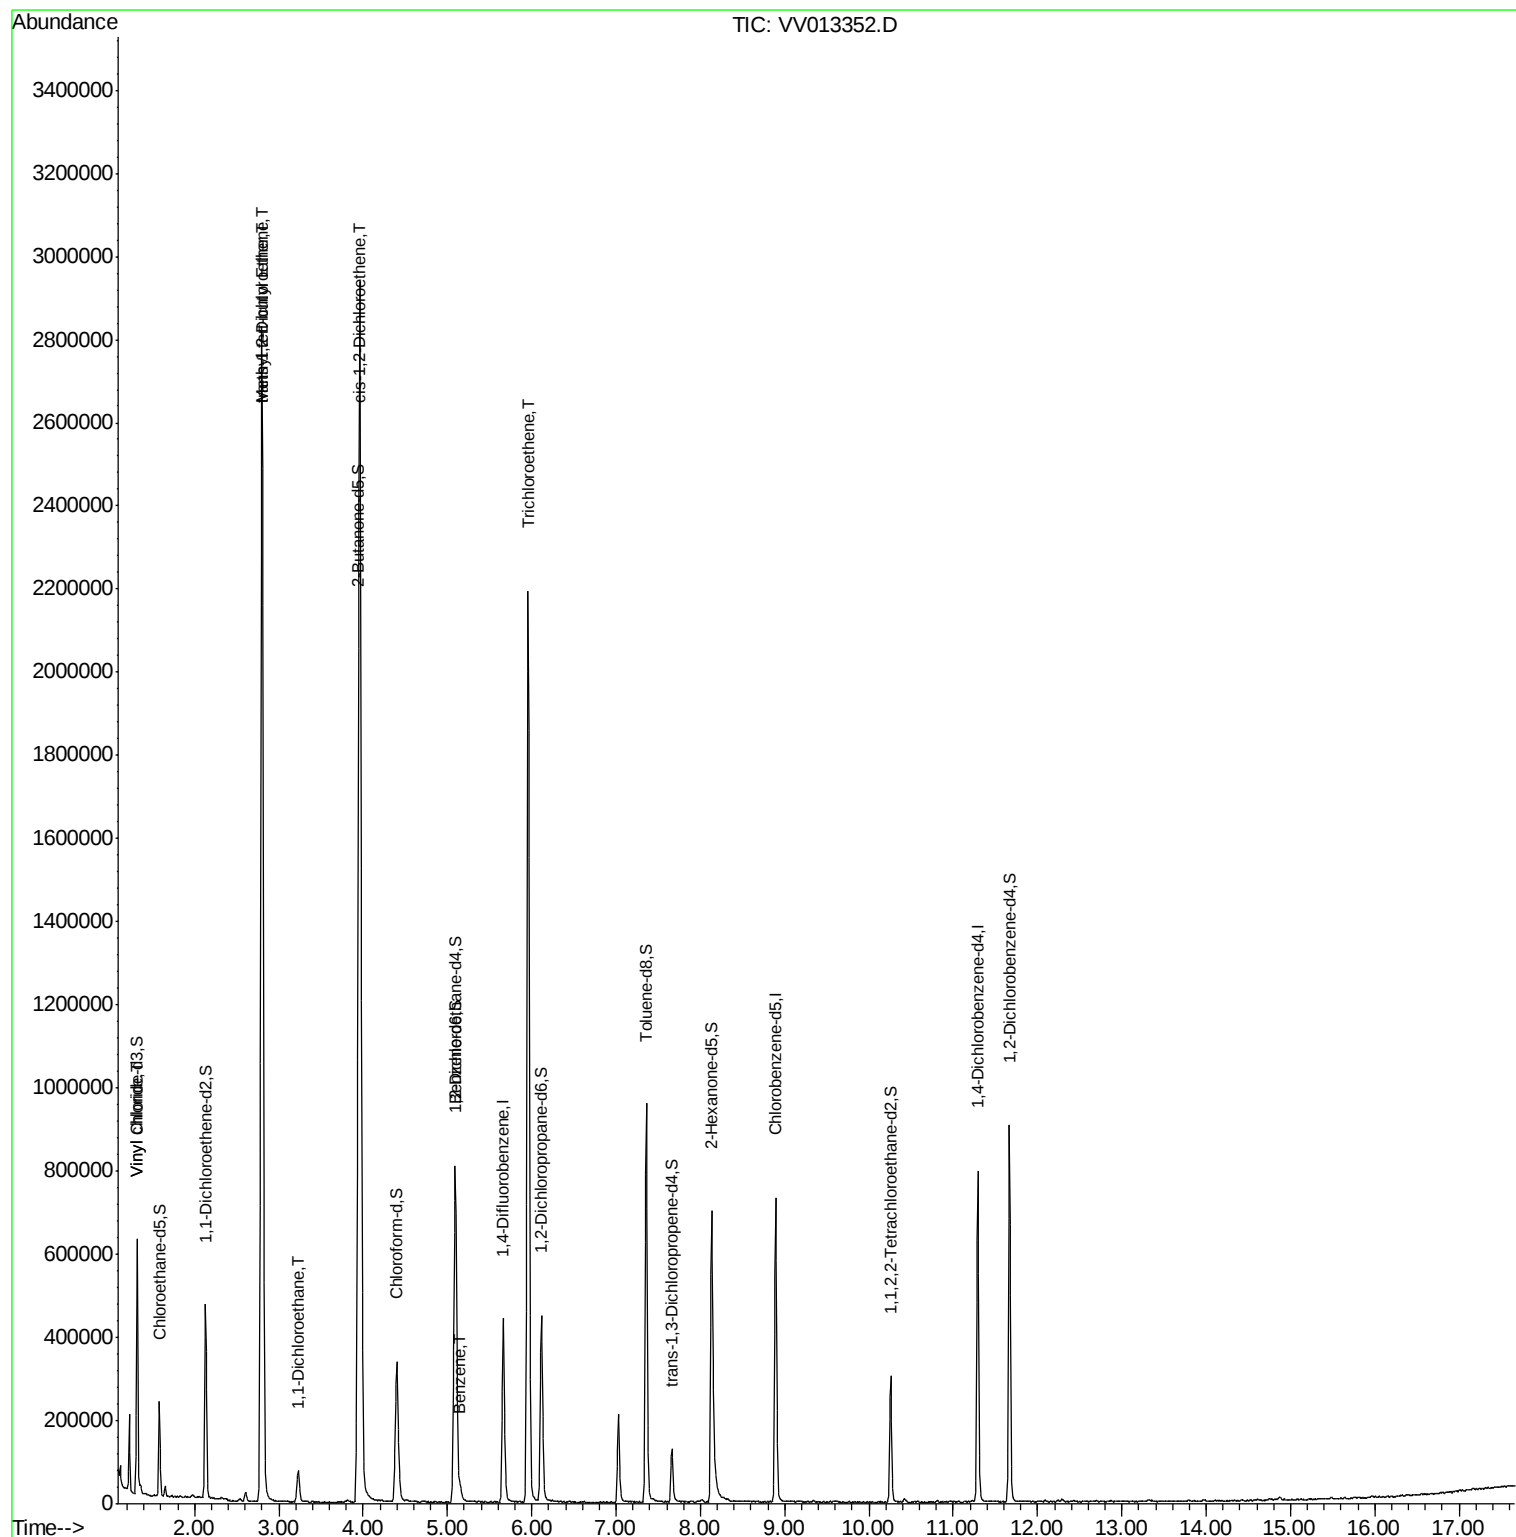

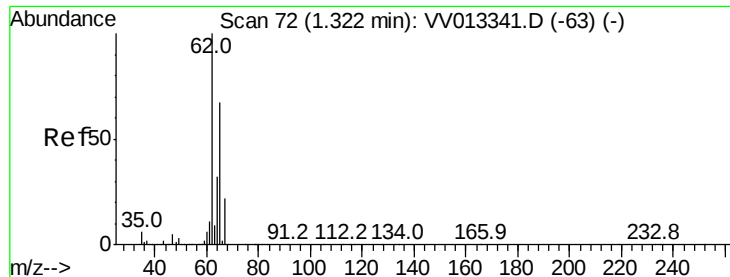

#5

Vinyl chloride

Concen: 3.753 ug/L

RT: 1.32 min Scan# 72

Delta R.T. 0.00 min

Lab File: VV013352.D

Acq: 25 Oct 2019 17:44

Instrument :

MSVOA_V

ClientSampleId :





H0G17

Tot Ion: 62 Resp: 145062

Ion Ratio Lower Upper

62 100

64 34.2 22.9 42.5

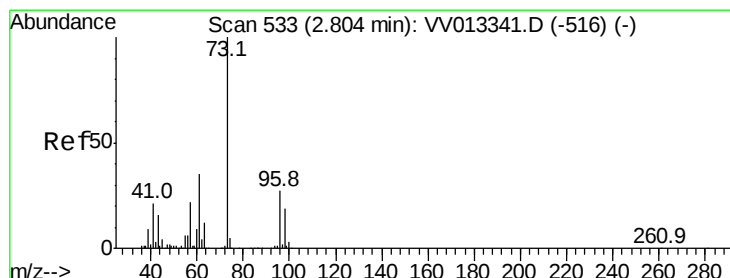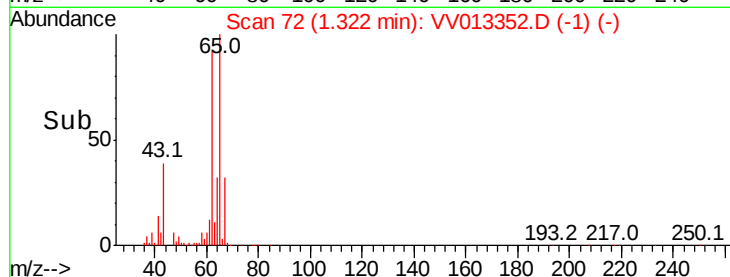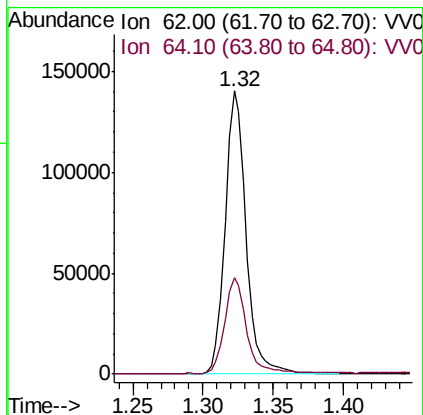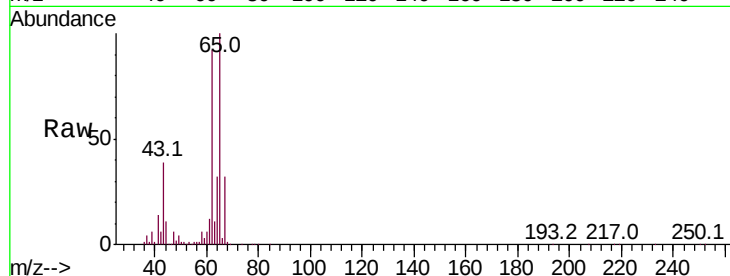

#17

Methyl tert-butyl Ether

Concen: 34.737 ug/L

RT: 2.80 min Scan# 532

Delta R.T. -0.00 min

Lab File: VV013352.D

Acq: 25 Oct 2019 17:44




Tgt Ion: 73 Resp: 2533046


Ion Ratio Lower Upper

73 100

43 17.2 13.1 19.7

57 22.1 16.4 24.6

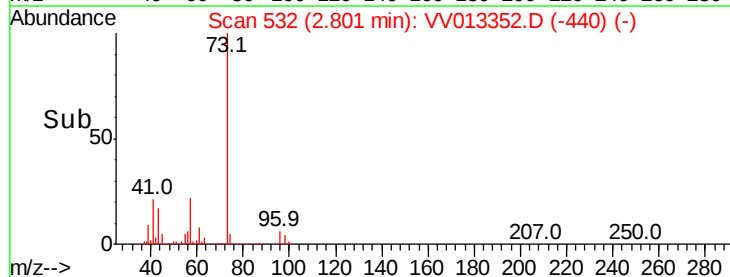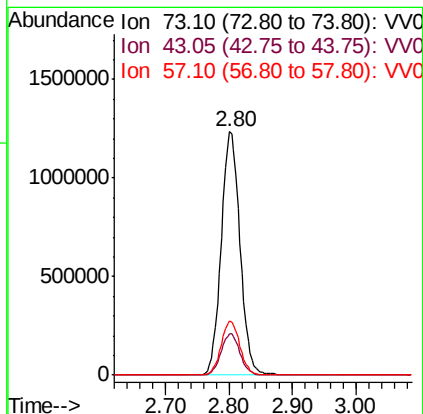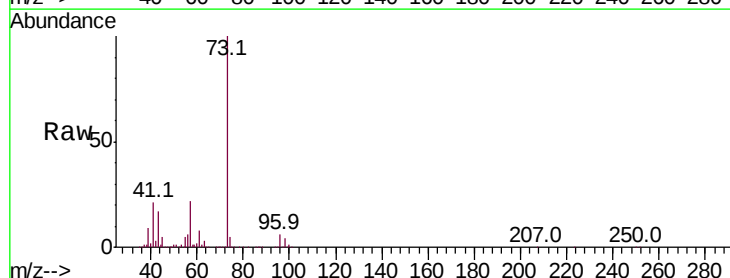

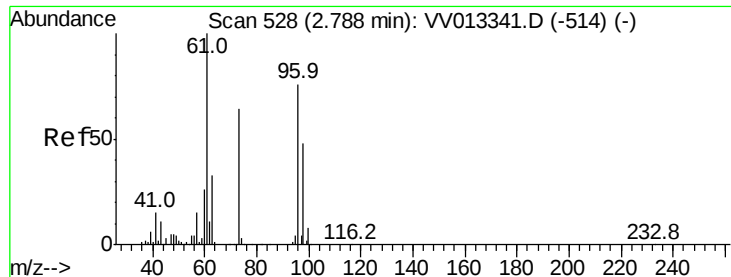

#18

trans-1,2-Dichloroethene

Concen: 4.784 ug/L

RT: 2.79 min Scan# 529

Delta R.T. 0.00 min

Lab File: VV013352.D

Acq: 25 Oct 2019 17:44

Instrument :

MSVOA_V

ClientSampleId :

H0G17


Tot Ion: 96 Resp: 177588

Ion Ratio Lower Upper

96 100

61 133.3 84.4 156.8




98 65.2 44.4 82.4

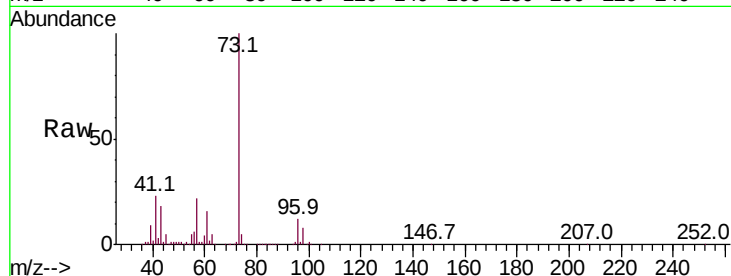

Abundance Ion 96.00 (95.70 to 96.70): VV0

Ion 61.05 (60.75 to 61.75): VV0

Ion 97.95 (97.65 to 98.65): VV0

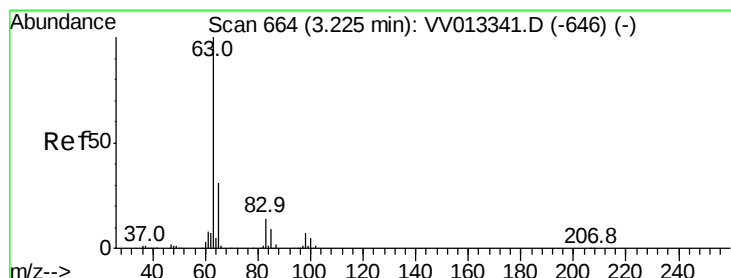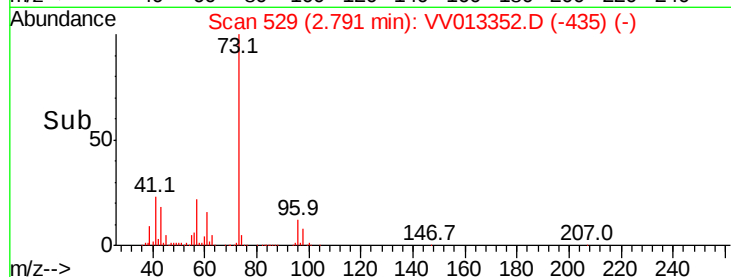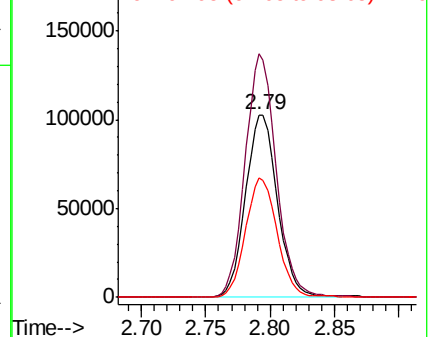

#19

1,1-Dichloroethane

Concen: 1.219 ug/L

RT: 3.23 min Scan# 665

Delta R.T. 0.00 min

Lab File: VV013352.D

Acq: 25 Oct 2019 17:44


Tgt Ion: 63 Resp: 73545

Ion Ratio Lower Upper

63 100

65 34.3 23.0 42.8



83 13.7 10.2 19.0

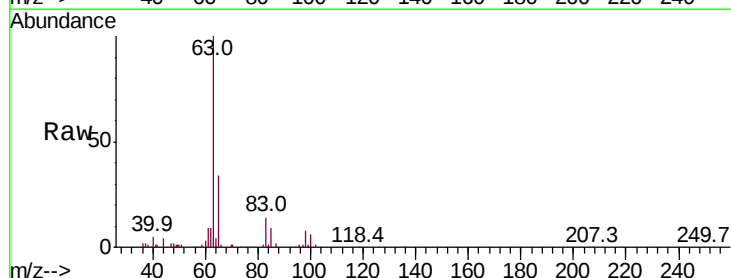


Abundance Ion 63.10 (62.80 to 63.80): VV0

Ion 65.10 (64.80 to 65.80): VV0

Ion 83.05 (82.75 to 83.75): VV0

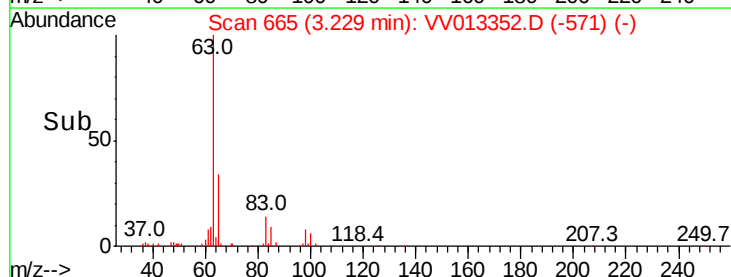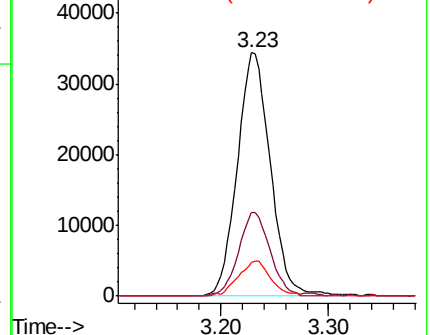




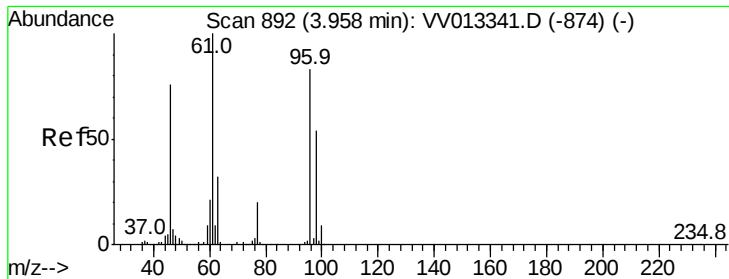


#22

cis-1,2-Dichloroethene
 Concen: 42.163 ug/L
 RT: 3.96 min Scan# 892
 Delta R.T. 0.00 min
 Lab File: VV013352.D
 Acq: 25 Oct 2019 17:44

Instrument :
 MSVOA_V
 ClientSampleId :
 H0G17




Tot Ion: 96 Resp: 1675062
 Ion Ratio Lower Upper
 96 100
 61 119.4 77.3 143.7
 68 0.0 0.1 0.1#

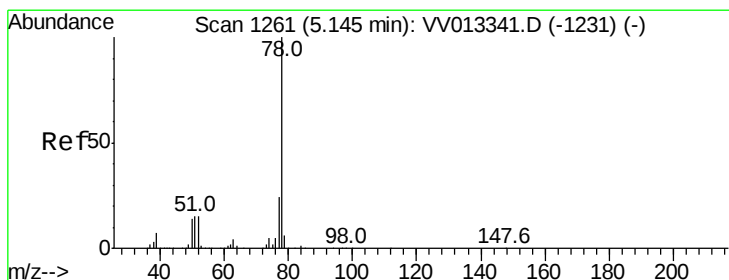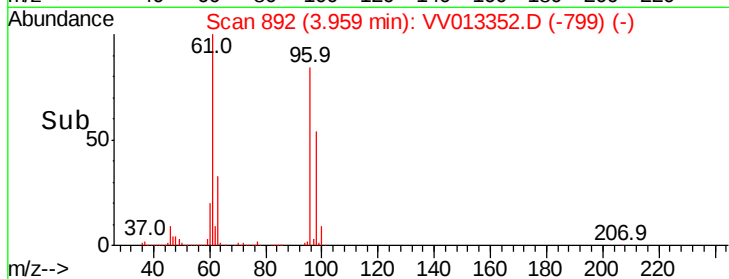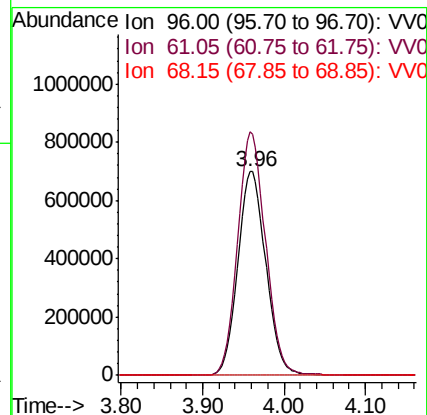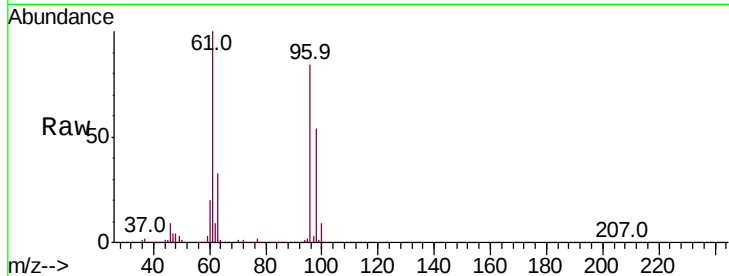


#33

Benzene
 Concen: 0.210 ug/L
 RT: 5.14 min Scan# 1261
 Delta R.T. 0.00 min
 Lab File: VV013352.D
 Acq: 25 Oct 2019 17:44

Tgt Ion: 78 Resp: 34858

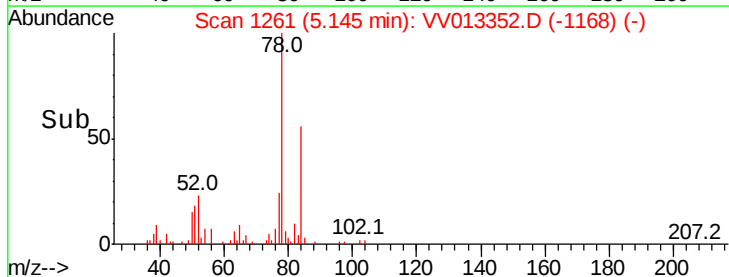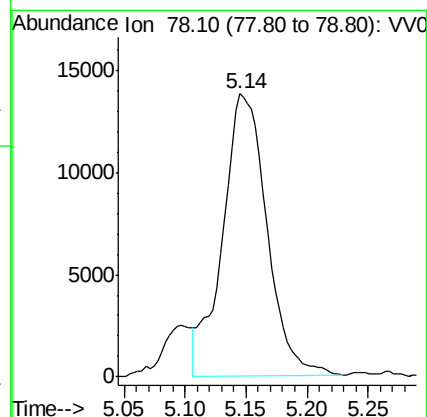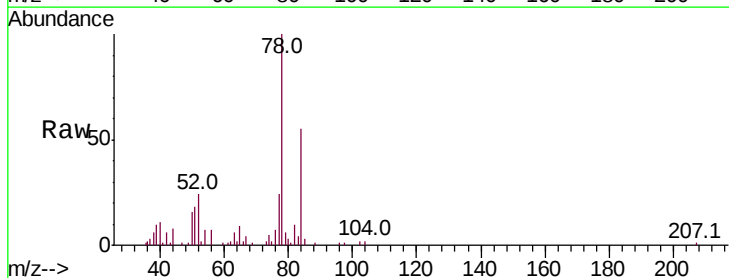

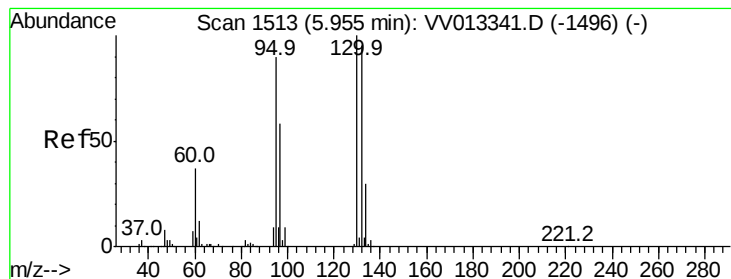

#34

Trichloroethene

Concen: 16.825 ug/L

RT: 5.96 min Scan# 1514

Delta R.T. 0.00 min

Lab File: VV013352.D

Acq: 25 Oct 2019 17:44

Instrument :
MSVOA_V
ClientSampleId :
H0G17

Tot Ion: 95 Resp: 747647



Ion Ratio Lower Upper

95 100

97 66.2 45.2 84.0

132 107.8 70.6 131.2

130 110.9 75.5 140.3

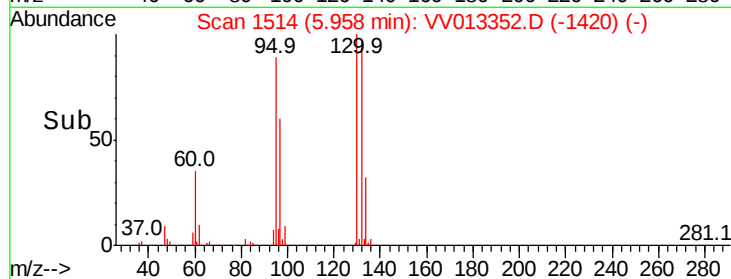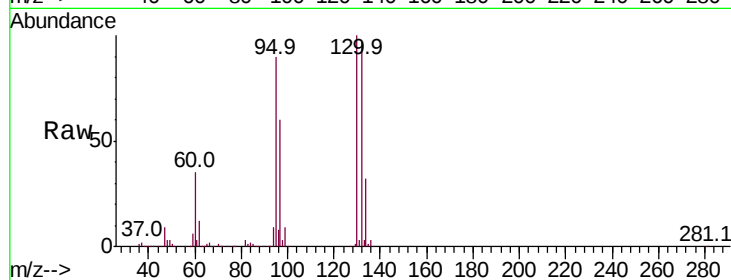

Abundance Ion 95.00 (94.70 to 95.70): VV0
Ion 96.95 (96.65 to 97.65): VV0
Ion 131.95 (131.65 to 132.65): V
Ion 129.95 (129.65 to 130.65): V

