


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102519\
 Data File : VV013340.D
 Acq On : 25 Oct 2019 12:14
 Operator : SY/MD
 Sample : BFB48
 Misc : 25.0ML/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB48

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Sat Oct 26 00:57:59 2019

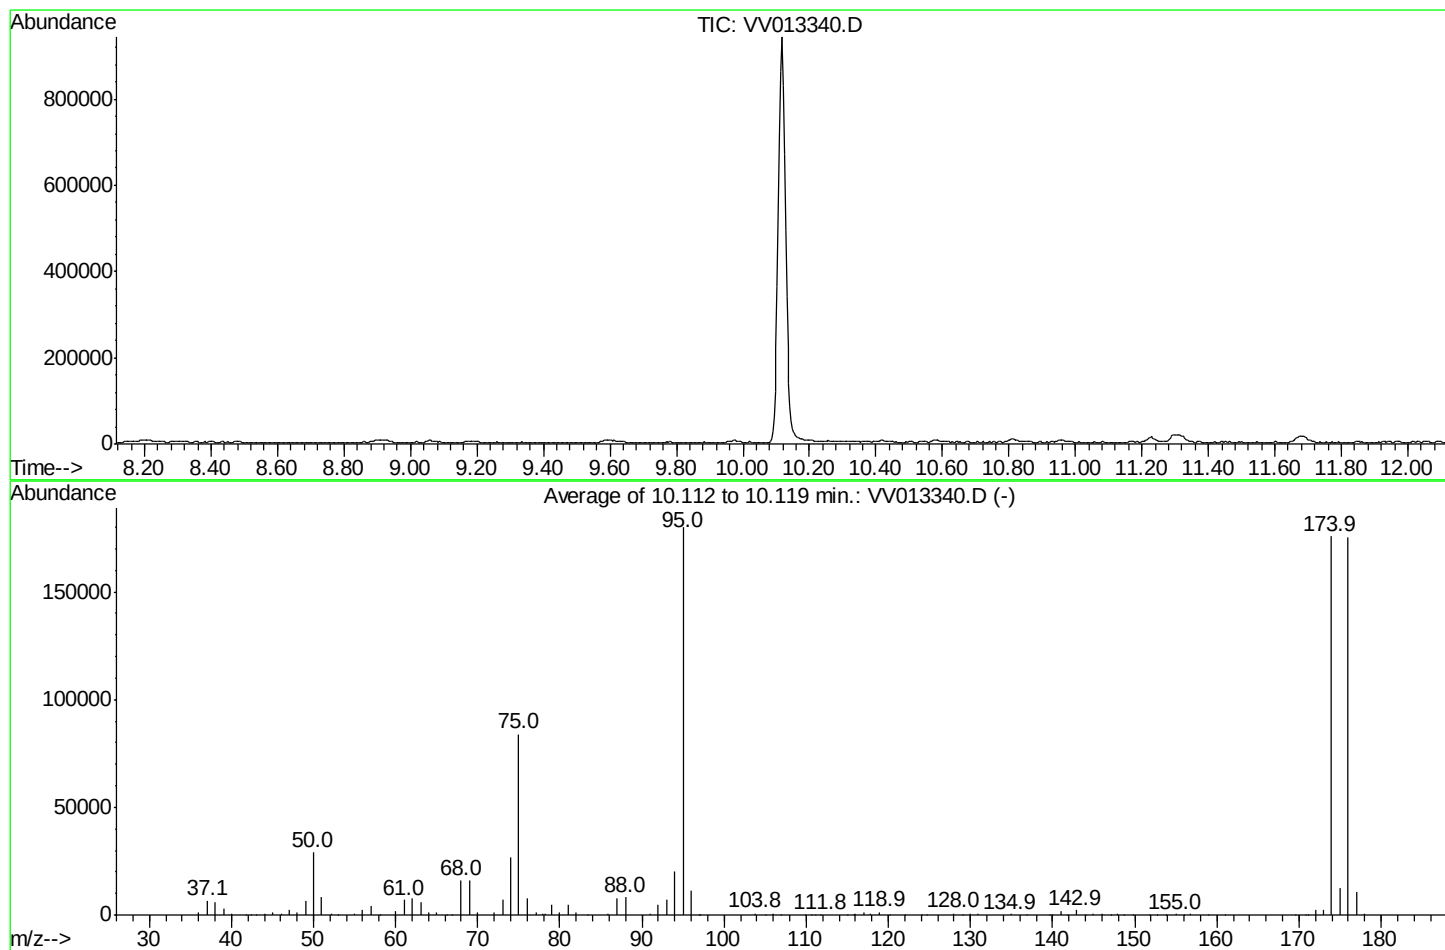

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.1	28896	PASS
75	95	30	80	46.6	83845	PASS
95	95	100	100	100.0	179925	PASS
96	95	5	9	6.2	11133	PASS
173	174	0.00	2	1.3	2237	PASS
174	95	50	120	97.7	175808	PASS
175	174	5	9	7.3	12751	PASS
176	174	95	101	99.6	175189	PASS
177	176	5	9	6.2	10916	PASS

Scan 2792 (10.067 min): VV013340.D
BFB48

m/z	Abundance
35.90	185.0
38.30	187.0
39.10	120.0
40.00	1099.0
44.00	1164.0
51.90	105.0
56.80	102.0
134.10	106.0
207.20	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	1240.0
37.10	6513.0
38.00	6456.0
39.10	2859.0
40.00	1584.0
42.30	126.0
42.90	231.0
44.00	1631.0
45.00	1353.0
46.00	266.0
47.00	2224.0
48.00	1081.0
49.00	5994.0
50.00	27592.0
51.00	8235.0
52.10	575.0
52.90	244.0
55.00	356.0
55.90	2146.0
57.10	3931.0
58.10	141.0
60.00	1535.0
61.00	6542.0
62.00	7183.0
63.10	5507.0
64.00	1130.0
65.00	1462.0
66.20	198.0
66.90	272.0
68.00	15519.0
69.00	15464.0
70.00	1308.0
71.90	884.0
73.00	7007.0
74.00	25296.0
75.00	80232.0
76.00	7325.0
77.10	902.0
77.90	462.0
78.20	465.0
79.00	4760.0
80.10	1239.0
80.90	4918.0
81.90	1312.0
85.80	488.0
87.00	7230.0
88.00	7684.0
91.00	684.0
92.00	4390.0
93.00	6945.0
94.00	18968.0
95.00	171392.0
96.10	10912.0
96.90	344.0
103.80	542.0
104.90	160.0
105.90	569.0
106.90	287.0
109.90	173.0
111.70	126.0
114.90	246.0
115.70	468.0
116.90	951.0
117.80	587.0
118.90	1280.0
120.20	120.0
124.70	112.0
128.00	681.0
129.00	289.0
130.00	592.0
130.90	311.0
135.00	319.0
136.70	300.0
139.60	124.0
141.00	1703.0
141.80	214.0
142.90	2116.0
144.00	149.0
144.80	812.0
145.90	379.0
147.20	151.0
147.90	454.0
148.70	124.0
149.70	220.0
153.80	139.0
155.00	516.0
156.00	153.0
156.80	326.0
159.00	122.0
160.90	224.0
170.80	307.0
172.00	2148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

173.00	2324.0
173.90	162432.0
175.00	12494.0
175.90	163968.0
177.00	10635.0
177.90	314.0
207.10	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.10	1398.0
37.10	6982.0
38.00	6419.0
39.00	3136.0
39.90	1429.0
42.30	133.0
43.00	247.0
44.00	2013.0
45.00	1448.0
46.10	371.0
47.00	2527.0
48.00	1047.0
49.00	6736.0
50.00	29832.0
51.00	8404.0
52.10	521.0
52.90	260.0
54.90	406.0
56.00	2376.0
57.10	4021.0
58.00	168.0
60.00	1678.0
61.00	7024.0
62.00	7854.0
63.10	6109.0
64.00	1266.0
65.00	1467.0
66.30	197.0
66.80	223.0
68.00	16592.0
69.00	16448.0
70.00	1271.0
72.00	984.0
73.00	7252.0
74.00	27688.0
75.00	86704.0
76.00	8011.0
77.10	947.0
78.20	618.0
79.00	5047.0
79.90	1346.0
80.90	5139.0
81.90	1390.0
83.30	119.0
85.80	342.0
86.90	7938.0
88.00	8619.0
90.90	674.0
92.00	4856.0
93.00	7372.0
94.00	20496.0
95.00	186240.0
96.10	11419.0
97.10	410.0
103.90	747.0
104.90	202.0
105.90	625.0
106.90	283.0
109.90	163.0
110.70	121.0
111.10	142.0
111.80	120.0
114.90	202.0
116.00	506.0
117.00	1043.0
117.80	632.0
118.90	1354.0
124.10	117.0
128.00	825.0
129.10	313.0
129.90	760.0
130.90	367.0
134.90	409.0
136.80	324.0
139.60	118.0
141.00	1747.0
141.90	236.0
142.90	2339.0
144.00	152.0
144.90	865.0
146.00	424.0
147.20	219.0
148.00	446.0
148.70	125.0
149.70	256.0
151.80	128.0
152.70	107.0
153.70	184.0
155.00	504.0
156.80	381.0
159.00	109.0
161.00	261.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

170.80	347.0
171.20	350.0
172.00	2452.0
173.10	2279.0
173.90	181184.0
175.00	13257.0
175.90	181120.0
177.00	11308.0
177.90	374.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.10	1461.0
37.10	6533.0
38.00	5785.0
39.00	3078.0
39.90	1350.0
41.80	127.0
42.30	109.0
42.90	244.0
44.00	2070.0
45.00	1275.0
46.10	366.0
47.00	2521.0
47.90	950.0
49.00	6593.0
50.00	29264.0
51.00	8185.0
52.20	479.0
52.90	279.0
54.90	462.0
56.00	2361.0
57.00	3730.0
58.00	203.0
60.00	1538.0
61.00	7068.0
62.00	7807.0
63.00	6065.0
64.00	1317.0
65.00	1354.0
66.30	135.0
66.80	272.0
68.00	15723.0
69.00	16165.0
70.00	1180.0
72.00	1038.0
73.00	6701.0
74.00	27752.0
75.00	84600.0
76.00	7612.0
77.10	1055.0
77.90	678.0
78.90	4826.0
79.90	1436.0
81.00	4959.0
81.90	1261.0
83.30	135.0
85.80	276.0
86.90	7812.0
88.00	8295.0
90.90	586.0
92.00	4843.0
93.00	7352.0
94.00	20816.0
95.00	182144.0
96.00	11069.0
97.10	502.0
103.90	926.0
105.00	247.0
105.90	606.0
107.00	238.0
109.90	102.0
110.70	189.0
111.10	170.0
111.80	161.0
115.00	185.0
116.00	611.0
117.00	1116.0
117.90	573.0
118.90	1115.0
122.00	122.0
124.10	160.0
127.90	841.0
129.00	333.0
129.90	862.0
130.90	391.0
134.80	453.0
136.90	299.0
139.90	145.0
141.00	1629.0
141.90	249.0
142.90	2364.0
144.00	138.0
144.90	889.0
146.00	459.0
147.10	205.0
148.00	459.0
148.70	113.0
149.70	229.0
151.80	126.0
152.70	201.0
153.70	171.0
155.00	464.0
156.80	451.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

158.90	121.0
160.90	277.0
169.60	118.0
171.10	451.0
172.00	2471.0
173.10	2110.0
173.90	183808.0
175.00	12504.0
175.90	180480.0
177.00	10805.0
178.00	352.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48