

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102521\
 Data File : VV023028.D
 Acq On : 25 Oct 2021 12:37
 Operator : SY/MD
 Sample : VV1025MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M

Title : VOC Analysis

Signal : TIC: VV023028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	119887	123636	14.61%	1.888%
2	1.568	156	164	174	rBV	82477	94855	11.21%	1.448%
3	2.031	306	308	313	rVB4	658	532	0.06%	0.008%
4	2.060	313	317	320	rBV2	545	492	0.06%	0.008%
5	2.108	320	332	342	rBV	139262	203147	24.01%	3.102%
6	2.288	382	388	397	rVB2	2226	3265	0.39%	0.050%
7	2.510	449	457	463	rBV4	2091	3260	0.39%	0.050%
8	2.613	487	489	496	rBV3	290	325	0.04%	0.005%
9	2.767	529	537	542	rVV4	982	1185	0.14%	0.018%
10	2.812	546	551	553	rBV	273	236	0.03%	0.004%
11	3.172	660	663	667	rBV3	291	290	0.03%	0.004%
12	3.310	702	706	709	rBV2	331	274	0.03%	0.004%
13	3.349	715	718	722	rVB3	429	362	0.04%	0.006%
14	3.378	722	727	729	rBV	329	355	0.04%	0.005%
15	3.908	882	892	923	rBV	33214	144990	17.14%	2.214%
16	4.349	1014	1029	1053	rBV2	128750	329322	38.93%	5.028%
17	4.651	1121	1123	1127	rBV4	357	252	0.03%	0.004%
18	4.748	1150	1153	1159	rBV4	416	418	0.05%	0.006%
19	4.828	1172	1178	1179	rBV3	499	432	0.05%	0.007%
20	5.047	1225	1246	1275	rBV2	326068	845960	100.00%	12.916%
21	5.291	1321	1322	1330	rVB2	805	647	0.08%	0.010%
22	5.330	1330	1334	1336	rBV5	405	317	0.04%	0.005%
23	5.384	1346	1351	1353	rBV3	375	320	0.04%	0.005%
24	5.397	1353	1355	1358	rBV3	705	382	0.05%	0.006%
25	5.484	1379	1382	1385	rBV2	674	398	0.05%	0.006%
26	5.503	1385	1388	1392	rVB4	598	392	0.05%	0.006%
27	5.526	1392	1395	1398	rBV3	510	340	0.04%	0.005%
28	5.548	1398	1402	1405	rVB3	622	502	0.06%	0.008%
29	5.564	1405	1407	1410	rBV2	559	309	0.04%	0.005%
30	5.619	1410	1424	1449	rBV	289693	586251	69.30%	8.951%
31	5.873	1499	1503	1504	rBV2	359	268	0.03%	0.004%
32	5.908	1504	1514	1530	rBV4	9835	22461	2.66%	0.343%
33	6.072	1552	1565	1586	rBV	181885	379686	44.88%	5.797%
34	6.407	1665	1669	1671	rBV2	368	254	0.03%	0.004%
35	6.648	1742	1744	1747	rVV2	438	326	0.04%	0.005%
36	6.680	1752	1754	1760	rVB4	679	570	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102521\
 Data File : VV023028.D
 Acq On : 25 Oct 2021 12:37
 Operator : SY/MD
 Sample : VV1025MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

37	6.751	1774	1776	1780	rBV2	346	258	0.03%	0.004%
38	6.883	1815	1817	1821	rVB3	348	238	0.03%	0.004%
39	6.934	1831	1833	1835	rBV3	559	260	0.03%	0.004%
40	6.989	1839	1850	1878	rVV	97714	185514	21.93%	2.832%
41	7.259	1930	1934	1935	rBV2	560	406	0.05%	0.006%
42	7.317	1940	1952	1970	rBV	375645	653608	77.26%	9.979%
43	7.625	2038	2048	2071	rBV	66903	120826	14.28%	1.845%
44	7.850	2111	2118	2120	rBV4	416	488	0.06%	0.007%
45	7.860	2120	2121	2126	rVB3	686	314	0.04%	0.005%
46	7.979	2154	2158	2160	rBV3	893	742	0.09%	0.011%
47	8.095	2181	2194	2225	rBV	188182	409319	48.39%	6.249%
48	8.320	2260	2264	2268	rVB5	484	437	0.05%	0.007%
49	8.362	2273	2277	2279	rBV3	658	552	0.07%	0.008%
50	8.374	2279	2281	2283	rVB3	599	252	0.03%	0.004%
51	8.641	2361	2364	2369	rBV4	753	535	0.06%	0.008%
52	8.854	2418	2430	2460	rBV	433807	707784	83.67%	10.806%
53	9.018	2479	2481	2484	rBV4	626	347	0.04%	0.005%
54	9.149	2516	2522	2525	rBV4	1689	1661	0.20%	0.025%
55	9.236	2547	2549	2554	rBV4	355	260	0.03%	0.004%
56	9.371	2586	2591	2594	rBV6	329	240	0.03%	0.004%
57	9.413	2602	2604	2608	rBV4	424	301	0.04%	0.005%
58	9.545	2642	2645	2646	rBV2	557	300	0.04%	0.005%
59	9.619	2663	2668	2673	rVB5	644	607	0.07%	0.009%
60	9.770	2711	2715	2718	rBV2	388	245	0.03%	0.004%
61	9.853	2738	2741	2744	rBV3	405	294	0.03%	0.004%
62	10.127	2817	2826	2834	rBV7	2261	4080	0.48%	0.062%
63	10.217	2843	2854	2877	rBV	256517	405612	47.95%	6.193%
64	10.352	2894	2896	2901	rVB4	864	690	0.08%	0.011%
65	10.384	2901	2906	2909	rBV4	899	794	0.09%	0.012%
66	10.410	2912	2914	2918	rVB2	500	335	0.04%	0.005%
67	10.545	2951	2956	2962	rVB6	1055	1424	0.17%	0.022%
68	10.583	2964	2968	2970	rVV4	758	520	0.06%	0.008%
69	10.599	2970	2973	2975	rVV2	740	391	0.05%	0.006%
70	10.799	3033	3035	3038	rBV2	465	247	0.03%	0.004%
71	10.918	3064	3072	3079	rBV6	3485	5331	0.63%	0.081%
72	11.040	3106	3110	3117	rVB4	594	597	0.07%	0.009%
73	11.143	3138	3142	3143	rBV3	1032	700	0.08%	0.011%
74	11.191	3152	3157	3164	rVB5	1869	2280	0.27%	0.035%
75	11.249	3164	3175	3192	rBV	421546	649816	76.81%	9.921%
76	11.429	3225	3231	3240	rVB6	2092	3082	0.36%	0.047%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102521\
 Data File : VV023028.D
 Acq On : 25 Oct 2021 12:37
 Operator : SY/MD
 Sample : VV1025MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis

77	11.468	3241	3243	3247	rVB3	735	334	0.04%	0.005%
78	11.535	3260	3264	3266	rBV3	898	554	0.07%	0.008%
79	11.625	3280	3292	3314	rBV	370549	586829	69.37%	8.960%
80	11.995	3405	3407	3412	rBV2	807	525	0.06%	0.008%
81	12.307	3501	3504	3511	rVB4	550	446	0.05%	0.007%
82	12.358	3517	3520	3527	rVB5	721	770	0.09%	0.012%
83	12.390	3527	3530	3531	rBV	388	254	0.03%	0.004%
84	12.432	3541	3543	3547	rVB2	561	350	0.04%	0.005%
85	12.522	3568	3571	3573	rBV2	457	275	0.03%	0.004%
86	12.648	3603	3610	3621	rBV3	5041	8090	0.96%	0.124%
87	12.699	3624	3626	3629	rBV2	613	444	0.05%	0.007%
88	12.831	3661	3667	3671	rBV2	567	692	0.08%	0.011%
89	12.995	3715	3718	3721	rBV3	397	357	0.04%	0.005%
90	13.268	3794	3803	3817	rVB3	6791	10231	1.21%	0.156%
91	13.329	3819	3822	3825	rBV	405	266	0.03%	0.004%
92	13.506	3869	3877	3889	rBV2	9384	15530	1.84%	0.237%
93	13.583	3897	3901	3906	rBV4	492	538	0.06%	0.008%
94	13.747	3944	3952	3962	rVB4	7235	11852	1.40%	0.181%
95	13.824	3974	3976	3979	rBV2	525	322	0.04%	0.005%
96	14.114	4061	4066	4071	rBV4	538	648	0.08%	0.010%
97	14.554	4200	4203	4208	rBV3	477	485	0.06%	0.007%
98	15.027	4347	4350	4351	rBV3	492	279	0.03%	0.004%
99	15.345	4447	4449	4454	rVB3	901	534	0.06%	0.008%
100	15.744	4571	4573	4576	rBV3	628	376	0.04%	0.006%




Sum of corrected areas: 6549679

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102521\
Data File : VV023028.D
Acq On : 25 Oct 2021 12:37
Operator : SY/MD
Sample : VV1025MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

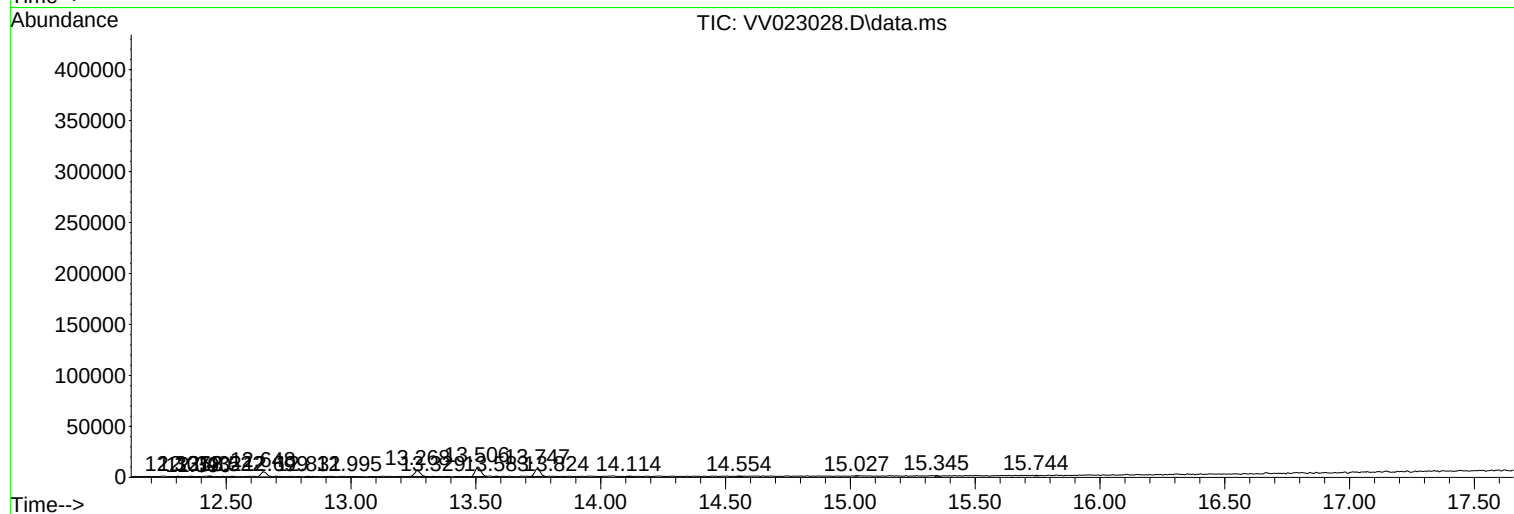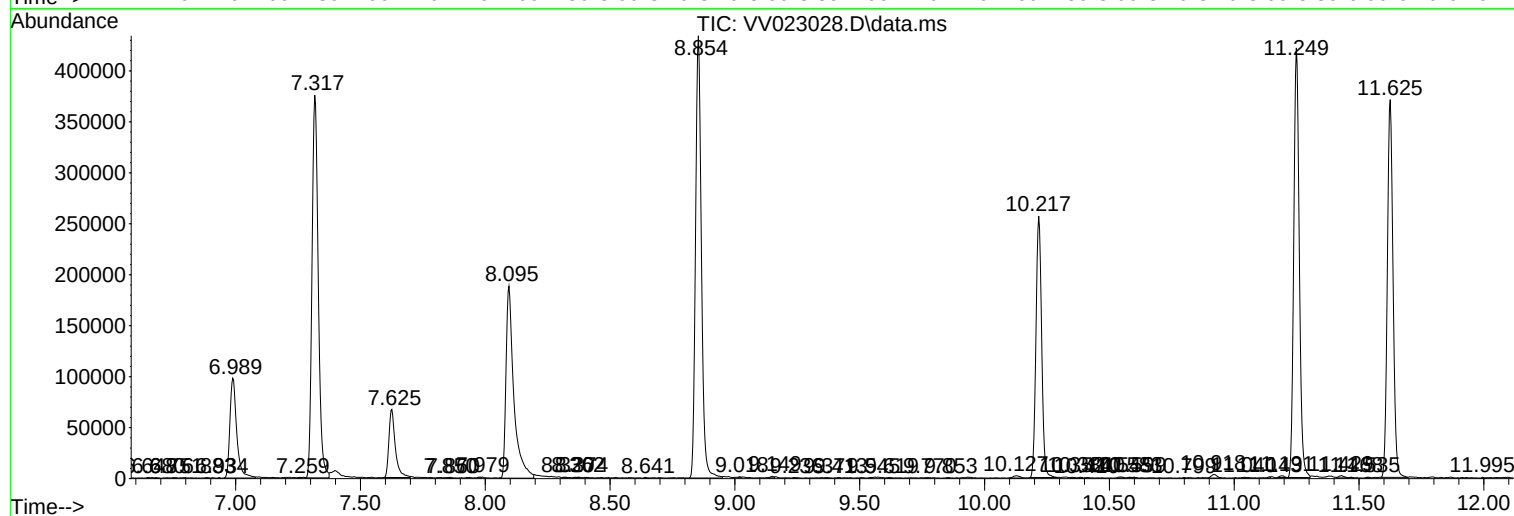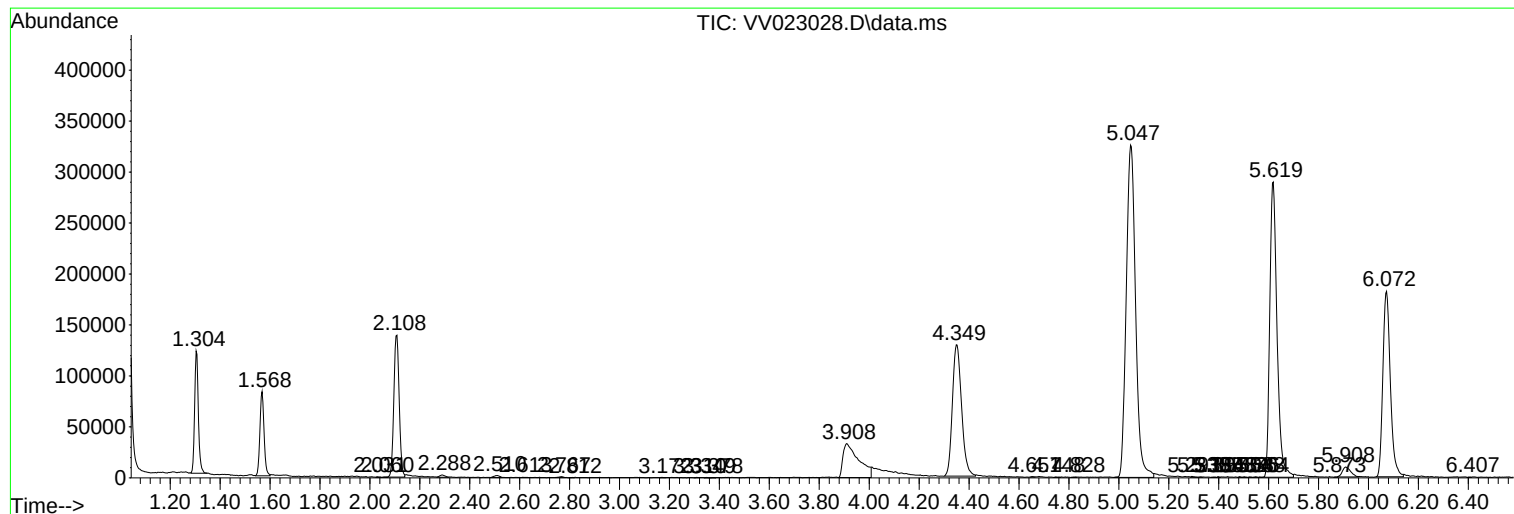

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102521\
Data File : VV023028.D
Acq On : 25 Oct 2021 12:37
Operator : SY/MD
Sample : VV1025MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102521\
Data File : VV023028.D
Acq On : 25 Oct 2021 12:37
Operator : SY/MD
Sample : VV1025MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
