
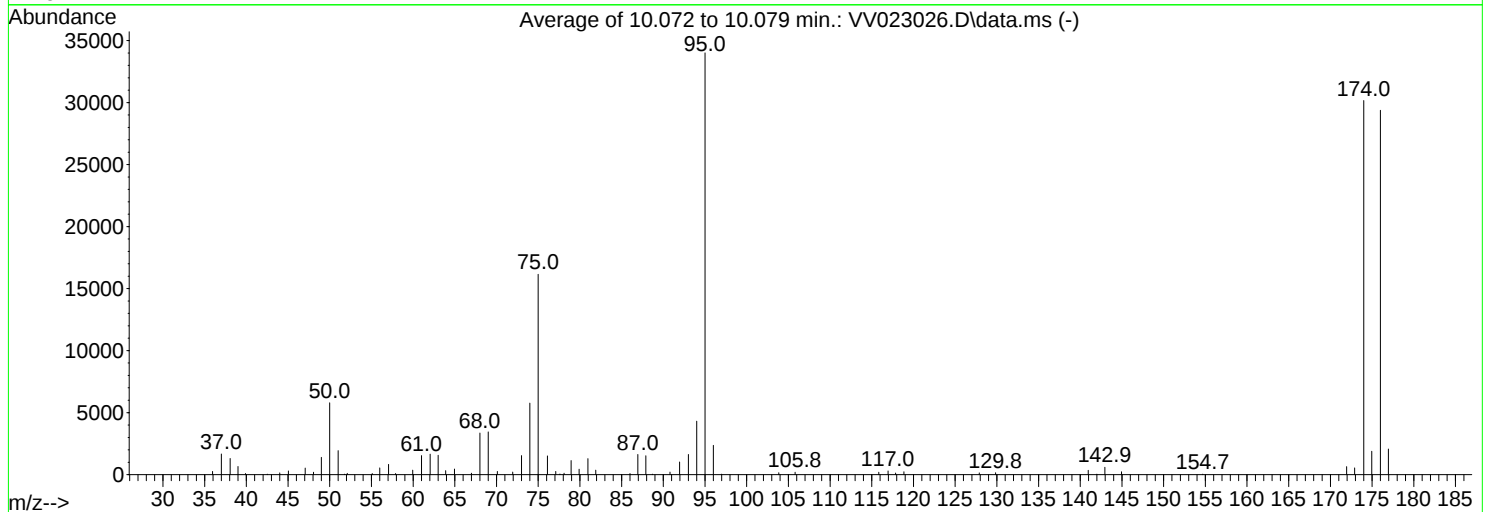


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102521\
 Data File : VV023026.D
 Acq On : 25 Oct 2021 09:26
 Operator : SY/MD
 Sample : BFB243
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB243

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100121WMA.M
 Title : VOC Analysis
 Last Update : Tue Oct 26 00:54:34 2021

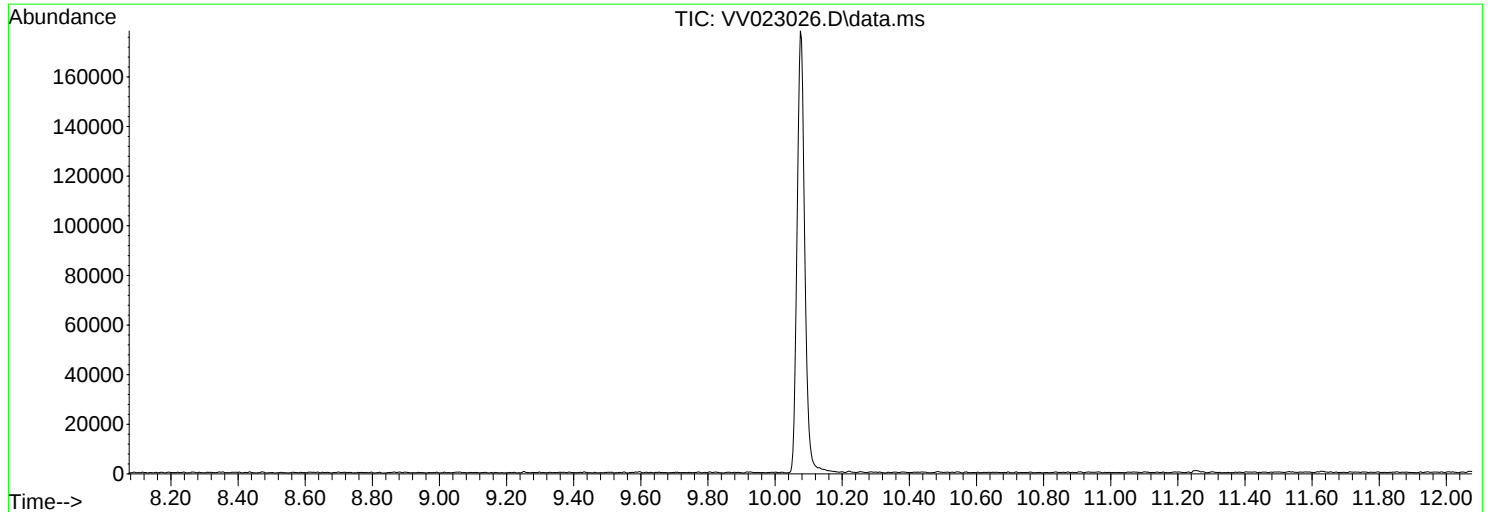

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	5792	PASS
75	95	30	80	47.5	16154	PASS
95	95	100	100	100.0	34013	PASS
96	95	5	9	7.0	2369	PASS
173	174	0.00	2	1.8	545	PASS
174	95	50	120	88.7	30160	PASS
175	174	5	9	6.2	1883	PASS
176	174	95	105	97.4	29379	PASS
177	176	5	10	7.0	2066	PASS

m/z	Abundance
39.90	191.0
44.00	262.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
35.90	263.0
37.00	1594.0
38.00	1215.0
39.00	697.0
39.90	302.0
44.00	385.0
45.00	279.0
47.10	593.0
48.00	210.0
49.00	1388.0
50.00	5699.0
51.00	1924.0
52.10	168.0
56.00	477.0
57.00	840.0
60.00	378.0
61.00	1520.0
62.10	1665.0
63.00	1420.0
63.90	295.0
65.00	451.0
66.90	120.0
68.00	3233.0
69.00	3198.0
70.10	290.0
71.90	228.0
73.00	1521.0
74.00	5689.0
75.00	15478.0
76.10	1480.0
77.10	294.0
78.10	176.0
78.90	1199.0
79.90	468.0
81.00	1292.0
81.90	315.0
86.00	123.0
87.00	1665.0
87.90	1438.0
90.80	206.0
92.00	1007.0
93.00	1659.0
94.00	4078.0
95.00	32400.0
96.00	2306.0
103.80	145.0
105.80	203.0
115.80	171.0
116.90	277.0
117.80	123.0
118.90	212.0
127.90	105.0
129.80	141.0
140.90	383.0
142.90	545.0
145.00	252.0
172.00	595.0
172.90	348.0
174.00	27864.0
174.90	1813.0
176.00	27640.0
176.90	1840.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
36.00	256.0
37.00	1718.0
38.00	1362.0
39.00	684.0
40.00	295.0
42.50	101.0
44.00	395.0
45.10	304.0
47.00	560.0
48.10	192.0
49.00	1454.0
50.00	5965.0
51.00	2011.0
52.10	160.0
55.10	111.0
56.00	549.0
57.10	843.0
57.90	126.0
59.90	361.0
61.00	1565.0
62.00	1735.0
63.00	1617.0
63.90	335.0
65.00	462.0
67.00	103.0
68.00	3456.0
69.00	3563.0
70.10	274.0
71.90	212.0
73.00	1562.0
74.00	5992.0
75.00	16720.0
76.10	1560.0
77.10	276.0
78.10	162.0
79.00	1161.0
79.90	458.0
81.00	1348.0
81.90	377.0
86.00	137.0
86.90	1669.0
87.90	1617.0
90.80	227.0
92.00	1060.0
93.00	1667.0
94.00	4492.0
95.00	35184.0
96.00	2446.0
103.80	160.0
105.80	202.0
115.80	222.0
116.90	306.0
117.90	128.0
118.90	233.0
127.90	155.0
129.80	157.0
140.90	361.0
142.00	102.0
142.90	600.0
144.90	242.0
171.90	661.0
172.80	423.0
174.00	31160.0
175.00	1906.0
176.00	30472.0
177.00	2131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243

m/z	Abundance
36.00	251.0
37.00	1667.0
38.10	1355.0
39.00	603.0
40.00	241.0
44.00	416.0
45.10	306.0
47.00	439.0
48.00	193.0
49.00	1326.0
50.00	5712.0
51.00	1889.0
51.80	123.0
55.10	159.0
56.00	587.0
57.00	788.0
57.90	158.0
59.90	350.0
61.00	1507.0
62.00	1564.0
63.00	1643.0
63.90	323.0
64.90	428.0
67.10	118.0
68.00	3388.0
69.00	3585.0
70.10	221.0
72.00	194.0
73.00	1508.0
74.00	5636.0
75.00	16263.0
76.10	1509.0
77.10	198.0
77.60	164.0
78.90	1056.0
79.90	389.0
80.90	1252.0
81.90	407.0
86.90	1547.0
87.90	1520.0
88.70	122.0
90.80	202.0
91.90	992.0
93.00	1539.0
94.00	4349.0
95.00	34456.0
96.00	2356.0
97.00	104.0
103.90	174.0
105.80	188.0
115.90	204.0
117.00	305.0
117.90	126.0
118.80	242.0
127.90	174.0
129.90	176.0
141.00	320.0
143.00	636.0
144.90	218.0
154.70	110.0
171.90	675.0
172.90	433.0
173.00	432.0
174.00	31456.0
175.00	1929.0
176.00	30024.0
177.00	2226.0

Instrument :
MSVOA_V
ClientSampleId :
BFB243