
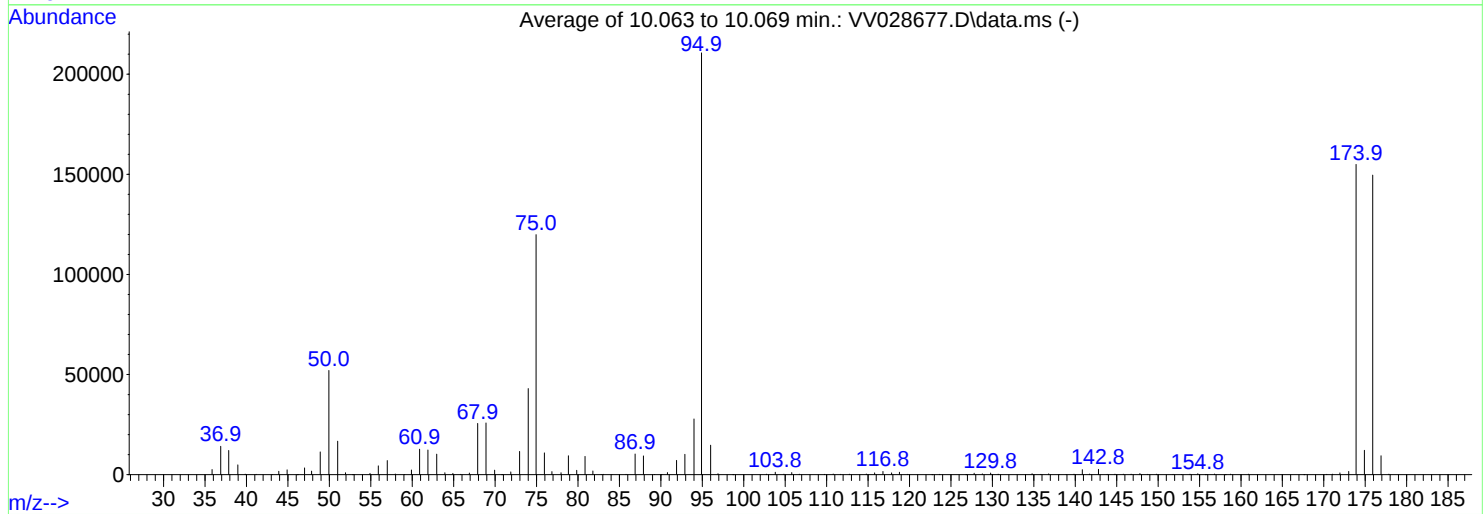


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102522\
 Data File : VV028677.D
 Acq On : 25 Oct 2022 09:05
 Operator : SY/MD
 Sample : BFB390
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB390

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Oct 28 21:50:06 2022

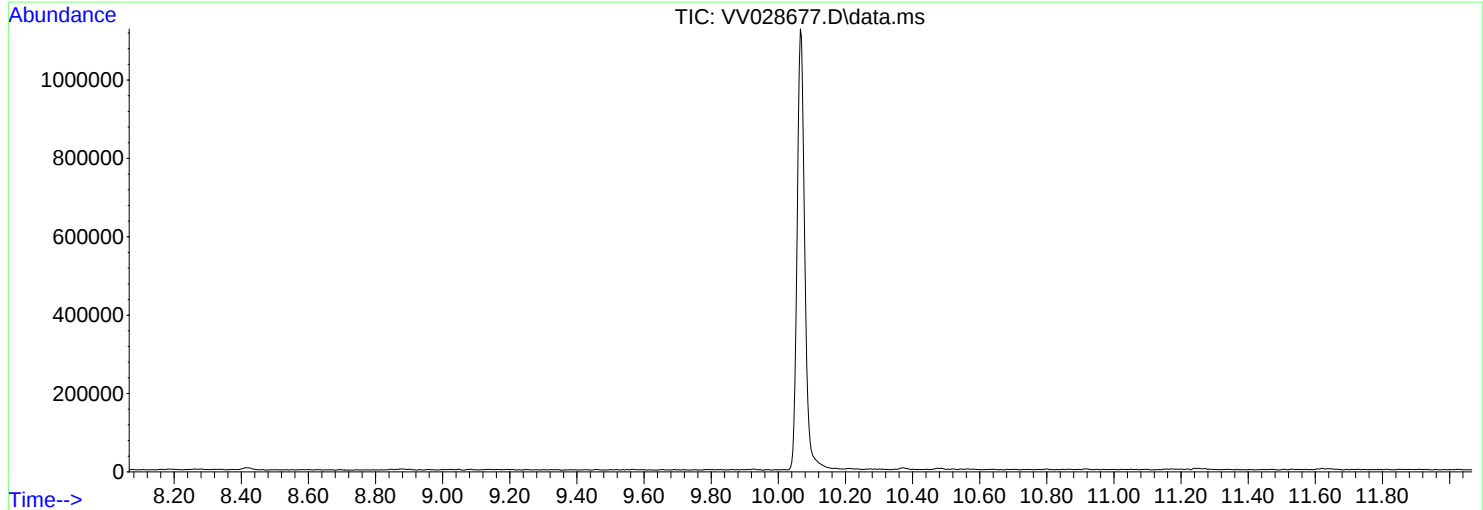

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2793

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.7	52045	PASS
75	95	30	80	56.9	119859	PASS
95	95	100	100	100.0	210688	PASS
96	95	5	9	7.0	14704	PASS
173	174	0.00	2	1.1	1638	PASS
174	95	50	120	73.5	154944	PASS
175	174	5	9	7.8	12152	PASS
176	174	95	105	96.6	149632	PASS
177	176	5	10	6.3	9450	PASS

m/z	Abundance
35.90	190.0
36.90	126.0
37.70	167.0
38.70	182.0
39.80	428.0
40.80	120.0
42.00	198.0
42.80	199.0
43.90	871.0
45.70	179.0
46.30	130.0
47.70	132.0
48.40	112.0
49.80	152.0
50.70	105.0
51.10	118.0
52.90	110.0
53.70	119.0
54.90	141.0
56.10	130.0
57.00	111.0
58.30	116.0
59.00	114.0
62.30	126.0
63.40	101.0
65.50	103.0
66.50	143.0
70.80	128.0
76.70	116.0
93.20	118.0
106.10	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
35.90	2640.0
36.90	13729.0
37.90	11921.0
38.90	4782.0
39.90	629.0
41.10	138.0
42.10	180.0
42.90	241.0
43.90	2452.0
44.90	2410.0
47.00	3094.0
47.90	1762.0
48.90	11195.0
50.00	49832.0
51.00	16291.0
52.00	975.0
52.80	157.0
54.90	813.0
55.90	4315.0
57.00	7024.0
57.90	360.0
59.10	139.0
59.90	2379.0
60.90	12092.0
61.90	12144.0
62.90	9910.0
63.90	886.0
64.90	529.0
65.80	119.0
66.90	798.0
67.90	24544.0
68.90	24768.0
69.90	2112.0
70.90	138.0
71.90	1250.0
72.90	11191.0
74.00	40824.0
75.00	114416.0
75.90	10421.0
76.90	1636.0
77.90	895.0
78.80	8943.0
79.90	2149.0
80.80	8796.0
81.80	1797.0
83.10	227.0
84.10	111.0
86.90	10012.0
87.90	8515.0
90.80	983.0
91.90	6934.0
92.90	9331.0
94.00	26912.0
94.90	199936.0
96.00	14000.0
96.90	500.0
98.70	109.0
102.70	192.0
103.80	1092.0
104.80	293.0
105.80	1062.0
106.80	231.0
109.70	183.0
110.80	250.0
111.70	166.0
112.70	204.0
114.80	353.0
115.80	802.0
116.80	1476.0
117.90	865.0
118.80	1166.0
119.80	126.0
123.70	156.0
127.80	761.0
128.80	386.0
129.80	711.0
130.70	239.0
134.00	124.0
134.80	451.0
135.80	121.0
136.80	356.0
138.10	109.0
138.90	121.0
139.90	245.0
140.90	2361.0
141.80	279.0
142.80	2617.0
143.80	208.0
144.80	265.0
145.80	237.0
146.80	176.0
147.80	507.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

148.80	157.0
149.80	243.0
151.90	158.0
152.80	101.0
153.80	189.0
154.80	519.0
155.70	119.0
156.80	328.0
158.70	191.0
160.90	289.0
170.40	154.0
171.10	262.0
172.00	912.0
173.00	2328.0
173.90	144192.0
174.90	11686.0
175.90	138304.0
176.90	8958.0
177.90	222.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
35.90	2812.0
36.90	14885.0
37.90	12626.0
39.00	5031.0
39.90	653.0
41.20	156.0
42.00	206.0
42.70	159.0
43.10	160.0
43.90	2660.0
44.90	2489.0
47.00	3483.0
47.90	2032.0
48.90	11663.0
50.00	54152.0
51.00	17456.0
52.00	967.0
52.70	151.0
52.90	161.0
54.90	821.0
55.90	4708.0
57.00	7364.0
57.90	317.0
59.10	175.0
59.90	2426.0
60.90	13243.0
61.90	12642.0
63.00	10631.0
64.00	1032.0
64.90	652.0
65.90	176.0
66.90	799.0
67.90	26608.0
68.90	26728.0
69.90	2318.0
70.90	164.0
71.90	1455.0
72.90	12076.0
74.00	44672.0
75.00	124312.0
76.00	11349.0
76.90	1730.0
78.00	939.0
78.90	9822.0
79.80	2255.0
80.80	9435.0
81.80	1909.0
83.00	203.0
84.10	116.0
85.80	237.0
86.90	10858.0
87.90	9619.0
89.30	104.0
90.80	1097.0
91.90	7377.0
92.90	10560.0
94.00	28768.0
94.90	218176.0
96.00	15370.0
96.90	531.0
102.70	245.0
103.80	1298.0
104.80	288.0
105.80	1103.0
106.70	266.0
109.80	189.0
110.80	330.0
111.70	185.0
112.80	264.0
114.80	319.0
115.80	911.0
116.80	1696.0
117.80	948.0
118.80	1250.0
119.80	150.0
123.60	181.0
127.80	768.0
128.80	430.0
129.80	791.0
130.70	246.0
134.00	123.0
134.80	452.0
135.90	144.0
136.80	371.0
138.00	103.0
138.90	131.0
139.90	243.0
140.80	2578.0
141.70	328.0
142.80	2741.0
143.80	182.0
144.80	240.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

145.80	271.0
146.80	221.0
147.80	614.0
148.80	142.0
149.80	311.0
151.80	182.0
152.80	132.0
153.90	207.0
154.80	532.0
155.90	124.0
156.80	332.0
158.80	266.0
160.90	237.0
170.40	163.0
171.00	291.0
172.00	983.0
173.00	2585.0
173.90	160256.0
174.90	12527.0
175.90	154752.0
176.90	9783.0
177.90	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
35.90	2700.0
37.00	14332.0
37.90	12059.0
39.00	4880.0
39.90	627.0
40.80	148.0
41.20	167.0
42.00	182.0
42.60	177.0
43.10	217.0
43.90	2679.0
44.90	2323.0
46.10	448.0
47.00	3429.0
47.90	1937.0
48.90	11204.0
50.00	52608.0
51.00	16744.0
51.90	865.0
53.00	145.0
54.90	704.0
55.90	4619.0
57.00	7079.0
58.00	283.0
59.10	203.0
59.90	2246.0
60.90	12900.0
61.90	12151.0
63.00	10253.0
64.00	1002.0
64.90	776.0
65.90	207.0
66.90	724.0
67.90	25488.0
68.90	26080.0
70.00	2338.0
70.90	205.0
71.90	1496.0
73.00	11591.0
74.00	43480.0
74.90	120848.0
76.00	10903.0
76.90	1479.0
78.00	997.0
78.90	9494.0
79.80	2143.0
80.90	9062.0
81.80	1909.0
82.80	236.0
85.80	276.0
86.90	10151.0
87.90	9937.0
89.20	107.0
90.00	112.0
90.80	1039.0
91.90	7083.0
92.90	10678.0
94.00	27688.0
94.90	213952.0
96.00	14743.0
96.90	474.0
102.80	271.0
103.80	1261.0
104.90	252.0
105.80	1046.0
106.60	265.0
109.80	187.0
110.80	396.0
111.70	203.0
112.80	305.0
114.80	245.0
115.80	936.0
116.80	1690.0
117.80	863.0
118.80	1216.0
119.80	136.0
122.70	114.0
123.60	188.0
126.80	127.0
127.80	740.0
128.80	402.0
129.80	834.0
130.70	239.0
134.00	104.0
134.80	449.0
135.90	133.0
136.80	399.0
138.90	123.0
139.70	236.0
140.80	2596.0
141.70	324.0
142.80	2613.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

143.90	170.0
144.80	224.0
145.80	299.0
146.70	235.0
147.80	664.0
148.70	117.0
149.80	299.0
151.70	196.0
152.80	144.0
153.90	228.0
154.80	487.0
156.00	163.0
156.80	337.0
158.10	102.0
158.80	311.0
160.90	214.0
167.60	119.0
170.30	162.0
171.00	246.0
171.90	853.0
173.90	160384.0
174.90	12243.0
175.90	155840.0
176.90	9609.0
177.80	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390