

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102618\
 Data File : VV008434.D
 Acq On : 26 Oct 2018 15:37
 Operator : SY/MD
 Sample : J5669-04
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBX1

Quant Time: Oct 27 05:29:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 27 04:42:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	196069	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	178184	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	71902	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	54388	50.10	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.20%
7) Chloroethane-d5	1.57	69	40765	52.01	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.02%
11) 1,1-Dichloroethene-d2	2.13	63	72989	37.23	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	74.46%
21) 2-Butanone-d5	3.93	46	114675	97.20	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.20%
24) Chloroform-d	4.41	84	125893	47.02	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.04%
26) 1,2-Dichloroethane-d4	5.09	65	88921	49.67	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.34%
32) Benzene-d6	5.10	84	263167	51.83	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.66%
36) 1,2-Dichloropropane-d6	6.12	67	89182	50.60	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.20%
41) Toluene-d8	7.36	98	236421	51.28	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	102.56%
43) trans-1,3-Dichloropropene-	7.67	79	42380	49.49	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.98%
47) 2-Hexanone-d5	8.14	63	85515	92.92	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	92.92%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	115637	48.44	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.88%
64) 1,2-Dichlorobenzene-d4	11.68	152	76371	51.92	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.84%


Target Compounds					Ovalue
13) Acetone	2.19	43	5354	5.847 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102618\
Data File : VV008434.D
Acq On : 26 Oct 2018 15:37
Operator : SY/MD
Sample : J5669-04
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBX1

Quant Time: Oct 27 05:29:27 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 27 04:42:32 2018
Response via : Initial Calibration

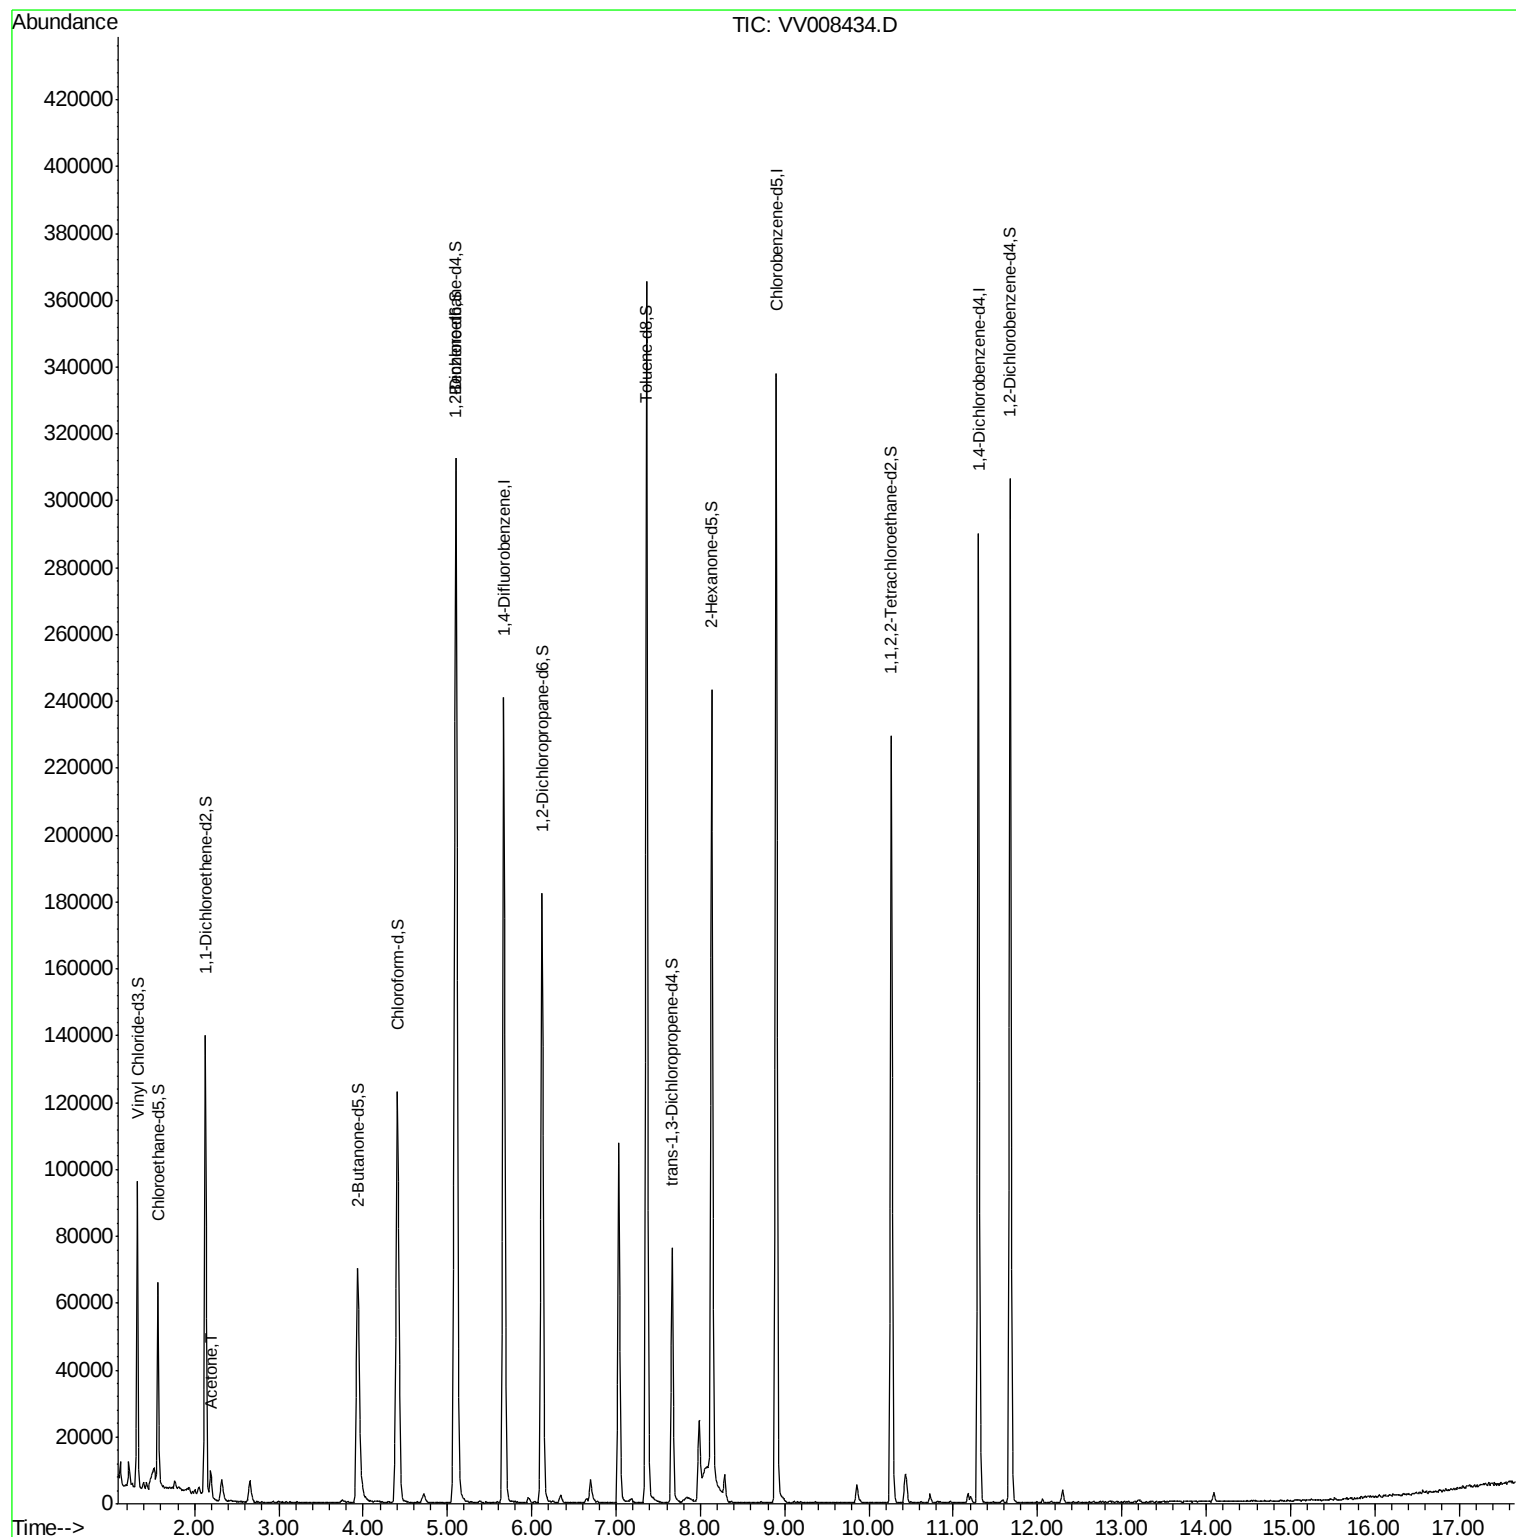

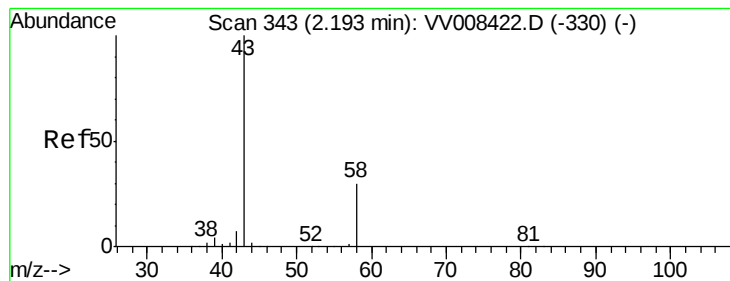

#13

Acetone

Concen: 5.847 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV008434.D

Acq: 26 Oct 2018 15:37

Instrument :
MSVOA_V
ClientSampleId :
ETBX1

Tot Ion: 43 Resp: 5354

Ion Ratio Lower Upper

43 100

58 33.8 0.0 61.4

