

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102618\
 Data File : VV008435.D
 Acq On : 26 Oct 2018 16:00
 Operator : SY/MD
 Sample : J5668-17
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBT9

Quant Time: Oct 27 05:32:29 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 27 04:42:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	191738	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	173389	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	71128	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	52233	49.20	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	98.40%
7) Chloroethane-d5	1.57	69	40528	52.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	105.74%
11) 1,1-Dichloroethene-d2	2.13	63	72208	37.66	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.32%
21) 2-Butanone-d5	3.94	46	112603	97.60	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	97.60%
24) Chloroform-d	4.41	84	126663	48.37	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.74%
26) 1,2-Dichloroethane-d4	5.09	65	88138	50.35	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.70%
32) Benzene-d6	5.11	84	258018	52.22	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	104.44%
36) 1,2-Dichloropropane-d6	6.12	67	86663	50.53	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	101.06%
41) Toluene-d8	7.36	98	232266	51.77	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.54%
43) trans-1,3-Dichloropropene-	7.67	79	41314	49.58	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	99.16%
47) 2-Hexanone-d5	8.14	63	84603	94.47	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	94.47%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	114483	49.29	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.58%
64) 1,2-Dichlorobenzene-d4	11.68	152	75384	51.81	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.62%


Target Compounds					Ovalue
13) Acetone	2.19	43	5400	6.031 ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102618\
Data File : VV008435.D
Acq On : 26 Oct 2018 16:00
Operator : SY/MD
Sample : J5668-17
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBT9

Quant Time: Oct 27 05:32:29 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 27 04:42:32 2018
Response via : Initial Calibration

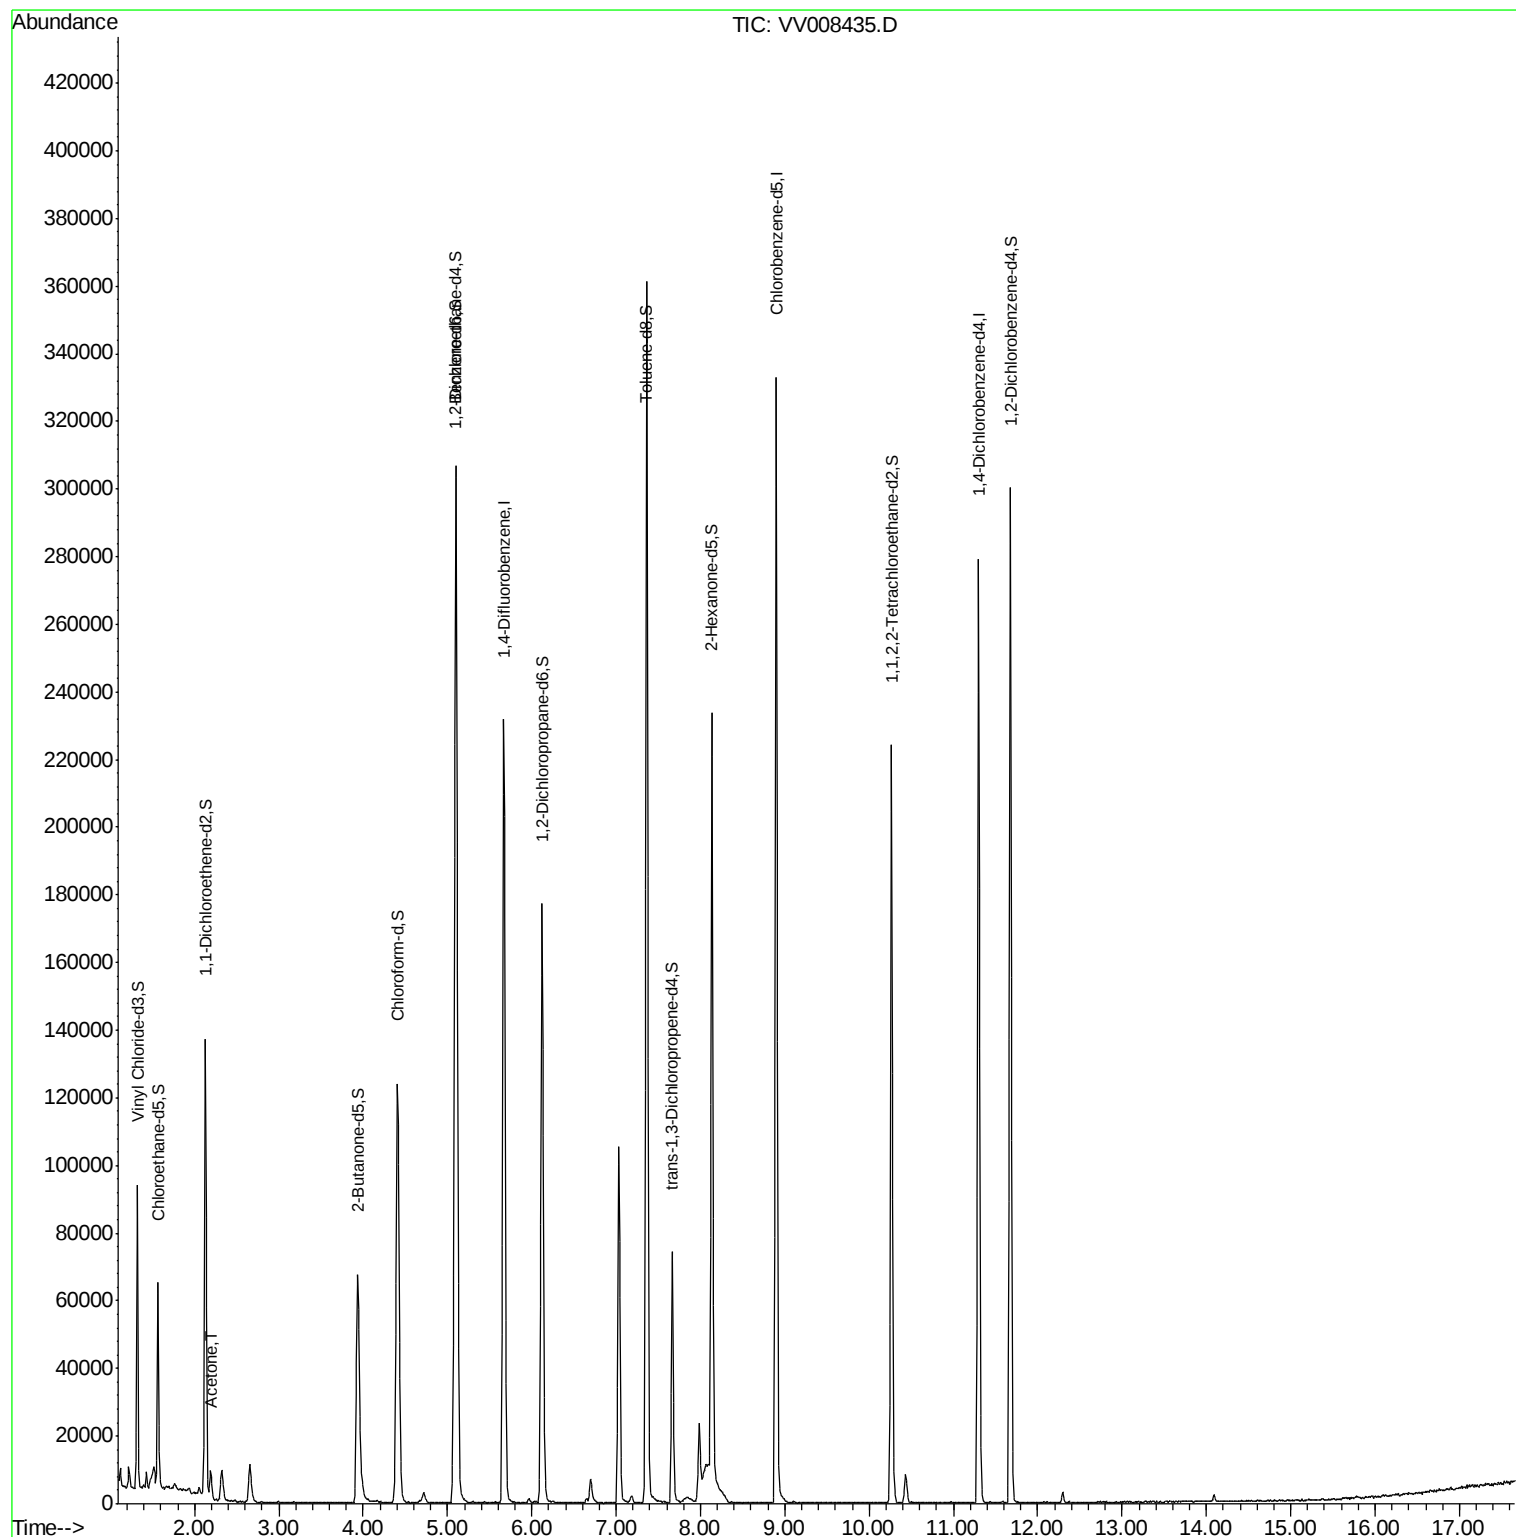

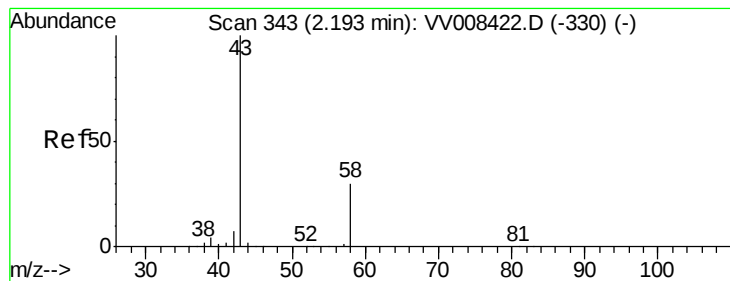

#13
 Acetone
 Concen: 6.031 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. -0.00 min
 Lab File: VV008435.D
 Acq: 26 Oct 2018 16:00

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBT9

Tot Ion: 43 Resp: 5400
 Ion Ratio Lower Upper
 43 100
 58 34.1 0.0 61.4

