

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102618\
 Data File : VV008436.D
 Acq On : 26 Oct 2018 16:23
 Operator : SY/MD
 Sample : J5668-16
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBT8

Quant Time: Oct 27 05:35:32 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Quant Title : VOC Analysis
 QLast Update : Sat Oct 27 04:42:32 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	190704	50.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	172470	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	69341	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	52987	50.18	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	100.36%
7) Chloroethane-d5	1.57	69	39732	52.12	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	104.24%
11) 1,1-Dichloroethene-d2	2.13	63	72239	37.88	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	75.76%
21) 2-Butanone-d5	3.93	46	109431	95.36	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	95.36%
24) Chloroform-d	4.41	84	124918	47.97	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.94%
26) 1,2-Dichloroethane-d4	5.09	65	87397	50.19	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	100.38%
32) Benzene-d6	5.10	84	254913	51.87	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	103.74%
36) 1,2-Dichloropropane-d6	6.12	67	87349	51.20	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	102.40%
41) Toluene-d8	7.36	98	231092	51.78	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	103.56%
43) trans-1,3-Dichloropropene-	7.67	79	40277	48.60	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	97.20%
47) 2-Hexanone-d5	8.14	63	81538	91.53	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	91.53%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	112269	48.59	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	97.18%
64) 1,2-Dichlorobenzene-d4	11.68	152	74260	52.35	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.70%


Target Compounds					Ovalue
13) Acetone	2.19	43	5268	5.915 ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102618\
Data File : VV008436.D
Acq On : 26 Oct 2018 16:23
Operator : SY/MD
Sample : J5668-16
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBT8

Quant Time: Oct 27 05:35:32 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis
QLast Update : Sat Oct 27 04:42:32 2018
Response via : Initial Calibration

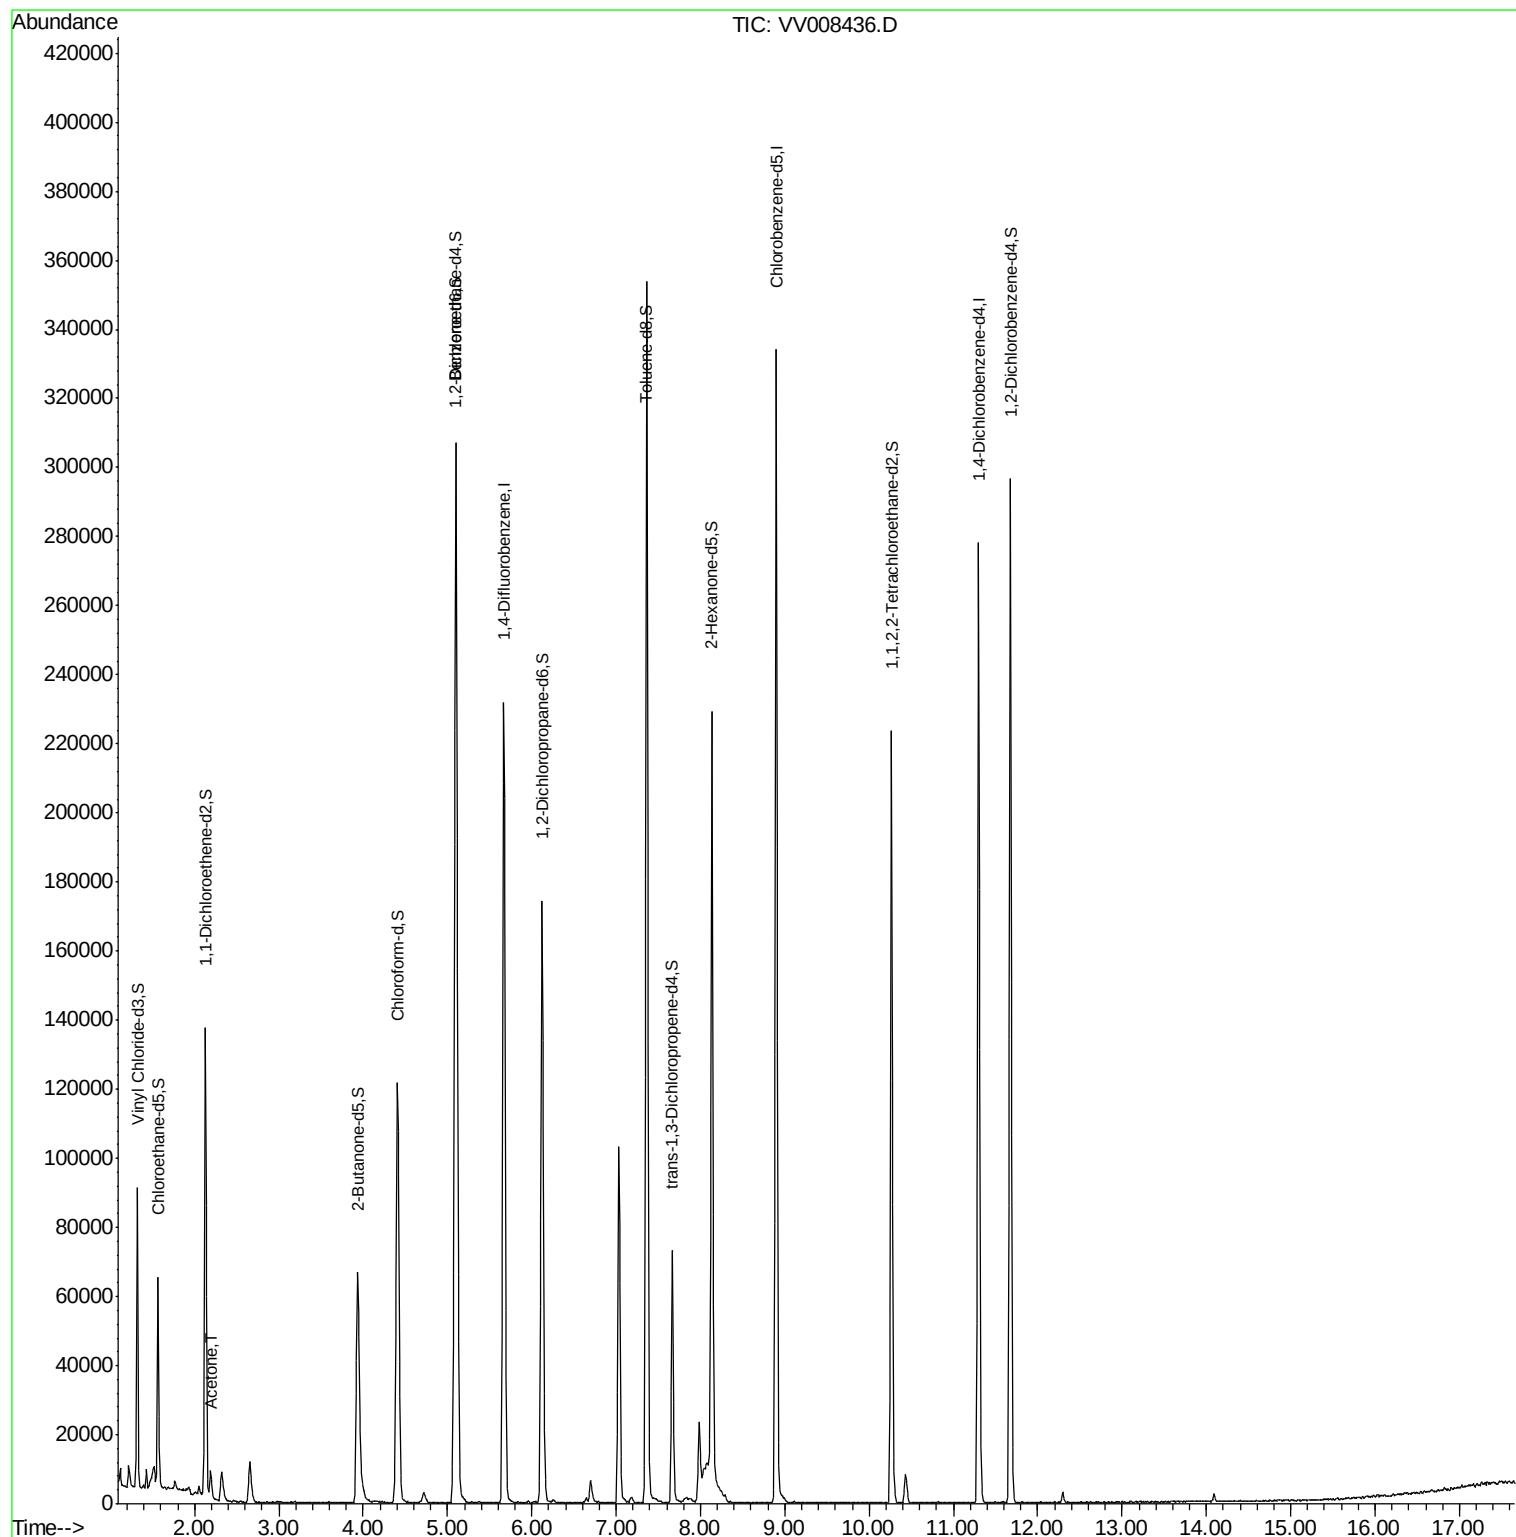

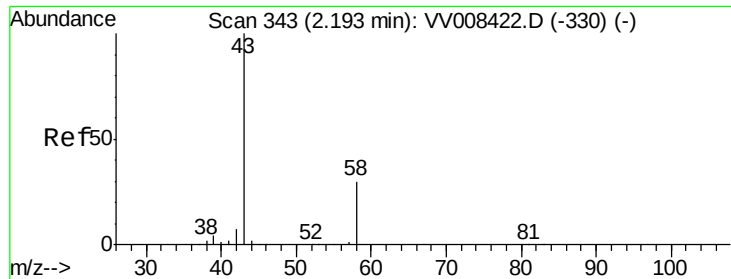

#13

Acetone

Concen: 5.915 ug/L

RT: 2.19 min Scan# 343

Delta R.T. 0.00 min

Lab File: VV008436.D

Acq: 26 Oct 2018 16:23

Instrument :
MSVOA_V
ClientSampleId :
ETBT8

Tot Ion: 43 Resp: 5268

Ion Ratio Lower Upper

43 100

58 28.9 0.0 61.4

