

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102618\
 Data File : VV008426.D
 Acq On : 26 Oct 2018 12:30
 Operator : SY/MD
 Sample : J5670-02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBP3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.216	34	39	50	rVB3	44882	47914	5.66%	0.711%
2	1.322	66	72	84	rVB	104802	108378	12.81%	1.608%
3	1.566	142	148	161	rVB	66504	80983	9.57%	1.202%
4	2.129	314	323	335	rBV	147715	206405	24.40%	3.063%
5	2.319	371	382	401	rBV	54088	112400	13.29%	1.668%
6	2.798	524	531	538	rVB3	2355	3875	0.46%	0.058%
7	2.991	583	591	592	rBV3	1031	1218	0.14%	0.018%
8	3.077	608	618	626	rBV4	1416	2399	0.28%	0.036%
9	3.110	626	628	632	rVB2	363	213	0.03%	0.003%
10	3.241	664	669	672	rBV2	325	294	0.03%	0.004%
11	3.312	688	691	695	rBV2	304	282	0.03%	0.004%
12	3.370	705	709	712	rBV	229	270	0.03%	0.004%
13	3.463	735	738	744	rBV2	149	155	0.02%	0.002%
14	3.798	837	842	845	rBV2	448	490	0.06%	0.007%
15	3.820	846	849	856	rVB4	741	652	0.08%	0.010%
16	3.852	856	859	866	rVB2	297	276	0.03%	0.004%
17	3.884	866	869	871	rBV	168	130	0.02%	0.002%
18	3.962	871	893	922	rBV2	92168	368251	43.53%	5.465%
19	4.267	984	988	991	rBV3	326	224	0.03%	0.003%
20	4.405	1009	1031	1063	rBV	133586	325398	38.46%	4.829%
21	4.527	1066	1069	1072	rBV2	367	301	0.04%	0.004%
22	4.624	1096	1099	1103	rBV2	299	267	0.03%	0.004%
23	4.720	1115	1129	1145	rVB3	3084	8520	1.01%	0.126%
24	4.839	1161	1166	1169	rBV2	211	175	0.02%	0.003%
25	4.945	1194	1199	1201	rBV2	378	173	0.02%	0.003%
26	4.965	1202	1205	1210	rVB3	292	254	0.03%	0.004%
27	5.100	1227	1247	1281	rBV2	337802	846020	100.00%	12.554%
28	5.309	1310	1312	1314	rBV2	342	134	0.02%	0.002%
29	5.335	1318	1320	1326	rVB3	324	261	0.03%	0.004%
30	5.360	1326	1328	1330	rBV	440	256	0.03%	0.004%
31	5.425	1346	1348	1352	rVB3	283	152	0.02%	0.002%
32	5.447	1352	1355	1358	rBV2	195	152	0.02%	0.002%
33	5.499	1366	1371	1374	rVB2	177	211	0.02%	0.003%
34	5.524	1374	1379	1381	rBV	286	254	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102618\
 Data File : VV008426.D
 Acq On : 26 Oct 2018 12:30
 Operator : SY/MD
 Sample : J5670-02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBP3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Title : VOC Analysis

35	5.669	1409	1424	1449	rBV	237057	462588	54.68%	6.864%
36	5.833	1473	1475	1478	rBV3	258	127	0.02%	0.002%
37	5.917	1496	1501	1502	rVB2	314	185	0.02%	0.003%
38	5.965	1502	1516	1533	rBV	144453	278014	32.86%	4.126%
39	6.122	1550	1565	1588	rBV	192699	384315	45.43%	5.703%
40	6.428	1657	1660	1663	rVB2	177	150	0.02%	0.002%
41	6.515	1682	1687	1690	rBV2	172	171	0.02%	0.003%
42	6.579	1704	1707	1709	rBV2	281	175	0.02%	0.003%
43	6.617	1715	1719	1722	rBV4	780	776	0.09%	0.012%
44	6.698	1737	1744	1762	rVB2	7010	14012	1.66%	0.208%
45	6.852	1790	1792	1794	rVV2	294	155	0.02%	0.002%
46	6.952	1821	1823	1825	rBV	225	129	0.02%	0.002%
47	7.032	1833	1848	1869	rBV2	117238	205925	24.34%	3.056%
48	7.187	1887	1896	1908	rVB5	8453	16165	1.91%	0.240%
49	7.248	1912	1915	1918	rBV2	255	166	0.02%	0.002%
50	7.280	1919	1925	1933	rBV6	1054	1642	0.19%	0.024%
51	7.363	1937	1951	1968	rBV	385520	668396	79.00%	9.918%
52	7.666	2033	2045	2063	rBV	80870	135662	16.04%	2.013%
53	7.762	2073	2075	2077	rBV3	381	177	0.02%	0.003%
54	7.984	2134	2144	2154	rBV	36026	71790	8.49%	1.065%
55	8.135	2183	2191	2213	rVB	244019	403084	47.64%	5.981%
56	8.334	2250	2253	2256	rBV2	215	152	0.02%	0.002%
57	8.678	2358	2360	2365	rVV	205	144	0.02%	0.002%
58	8.762	2383	2386	2389	rBV	223	213	0.03%	0.003%
59	8.813	2398	2402	2403	rBV	209	154	0.02%	0.002%
60	8.897	2415	2428	2447	rBV	330866	540590	63.90%	8.022%
61	9.058	2476	2478	2486	rVB2	471	446	0.05%	0.007%
62	9.174	2507	2514	2515	rBV4	2090	1926	0.23%	0.029%
63	9.228	2525	2531	2534	rBV	219	192	0.02%	0.003%
64	9.495	2610	2614	2616	rBV2	185	173	0.02%	0.003%
65	9.572	2634	2638	2639	rBV2	376	185	0.02%	0.003%
66	9.595	2639	2645	2652	rVB3	1105	1562	0.18%	0.023%
67	9.804	2705	2710	2713	rBV2	173	181	0.02%	0.003%
68	9.826	2713	2717	2718	rBV	169	138	0.02%	0.002%
69	9.865	2725	2729	2730	rBV	283	183	0.02%	0.003%
70	10.064	2783	2791	2797	rBV5	956	1353	0.16%	0.020%
71	10.129	2806	2811	2814	rVB	264	262	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102618\
 Data File : VV008426.D
 Acq On : 26 Oct 2018 12:30
 Operator : SY/MD
 Sample : J5670-02
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETBP3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Title : VOC Analysis

72	10.264	2842	2853	2871	rBV	241514	384860	45.49%	5.711%
73	10.350	2876	2880	2884	rBV	212	148	0.02%	0.002%
74	10.379	2888	2889	2893	rVB	308	149	0.02%	0.002%
75	10.434	2893	2906	2920	rBV3	12440	28409	3.36%	0.422%
76	10.582	2949	2952	2960	rBV3	594	674	0.08%	0.010%
77	10.621	2962	2964	2966	rVB2	440	216	0.03%	0.003%
78	10.643	2966	2971	2973	rBV	210	178	0.02%	0.003%
79	10.961	3063	3070	3075	rBV4	924	1324	0.16%	0.020%
80	11.013	3083	3086	3088	rBV	396	204	0.02%	0.003%
81	11.061	3098	3101	3102	rBV	319	148	0.02%	0.002%
82	11.196	3139	3143	3147	rBV2	271	274	0.03%	0.004%
83	11.299	3163	3175	3196	rBV	290848	465552	55.03%	6.908%
84	11.456	3221	3224	3227	rBV	271	142	0.02%	0.002%
85	11.582	3252	3263	3274	rBV4	2095	3868	0.46%	0.057%
86	11.675	3280	3292	3314	rVB	332358	533708	63.08%	7.920%
87	11.826	3336	3339	3342	rBV3	385	306	0.04%	0.005%
88	12.048	3405	3408	3410	rBV2	207	146	0.02%	0.002%
89	12.109	3423	3427	3429	rBV2	211	165	0.02%	0.002%
90	12.183	3447	3450	3453	rBV2	259	243	0.03%	0.004%
91	12.254	3469	3472	3474	rBV	352	158	0.02%	0.002%
92	12.296	3479	3485	3495	rVB2	5106	7351	0.87%	0.109%
93	12.360	3499	3505	3506	rBV2	224	225	0.03%	0.003%
94	12.659	3595	3598	3602	rBV2	169	174	0.02%	0.003%
95	12.890	3668	3670	3672	rBV	341	208	0.02%	0.003%
96	13.164	3752	3755	3758	rBV2	396	228	0.03%	0.003%
97	13.308	3797	3800	3803	rBV2	330	196	0.02%	0.003%
98	13.363	3814	3817	3821	rBV	246	183	0.02%	0.003%
99	13.427	3834	3837	3838	rBV2	393	205	0.02%	0.003%
100	13.463	3844	3848	3851	rBV2	296	254	0.03%	0.004%


Sum of corrected areas: 6738891

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102618\
Data File : VV008426.D
Acq On : 26 Oct 2018 12:30
Operator : SY/MD
Sample : J5670-02
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBP3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

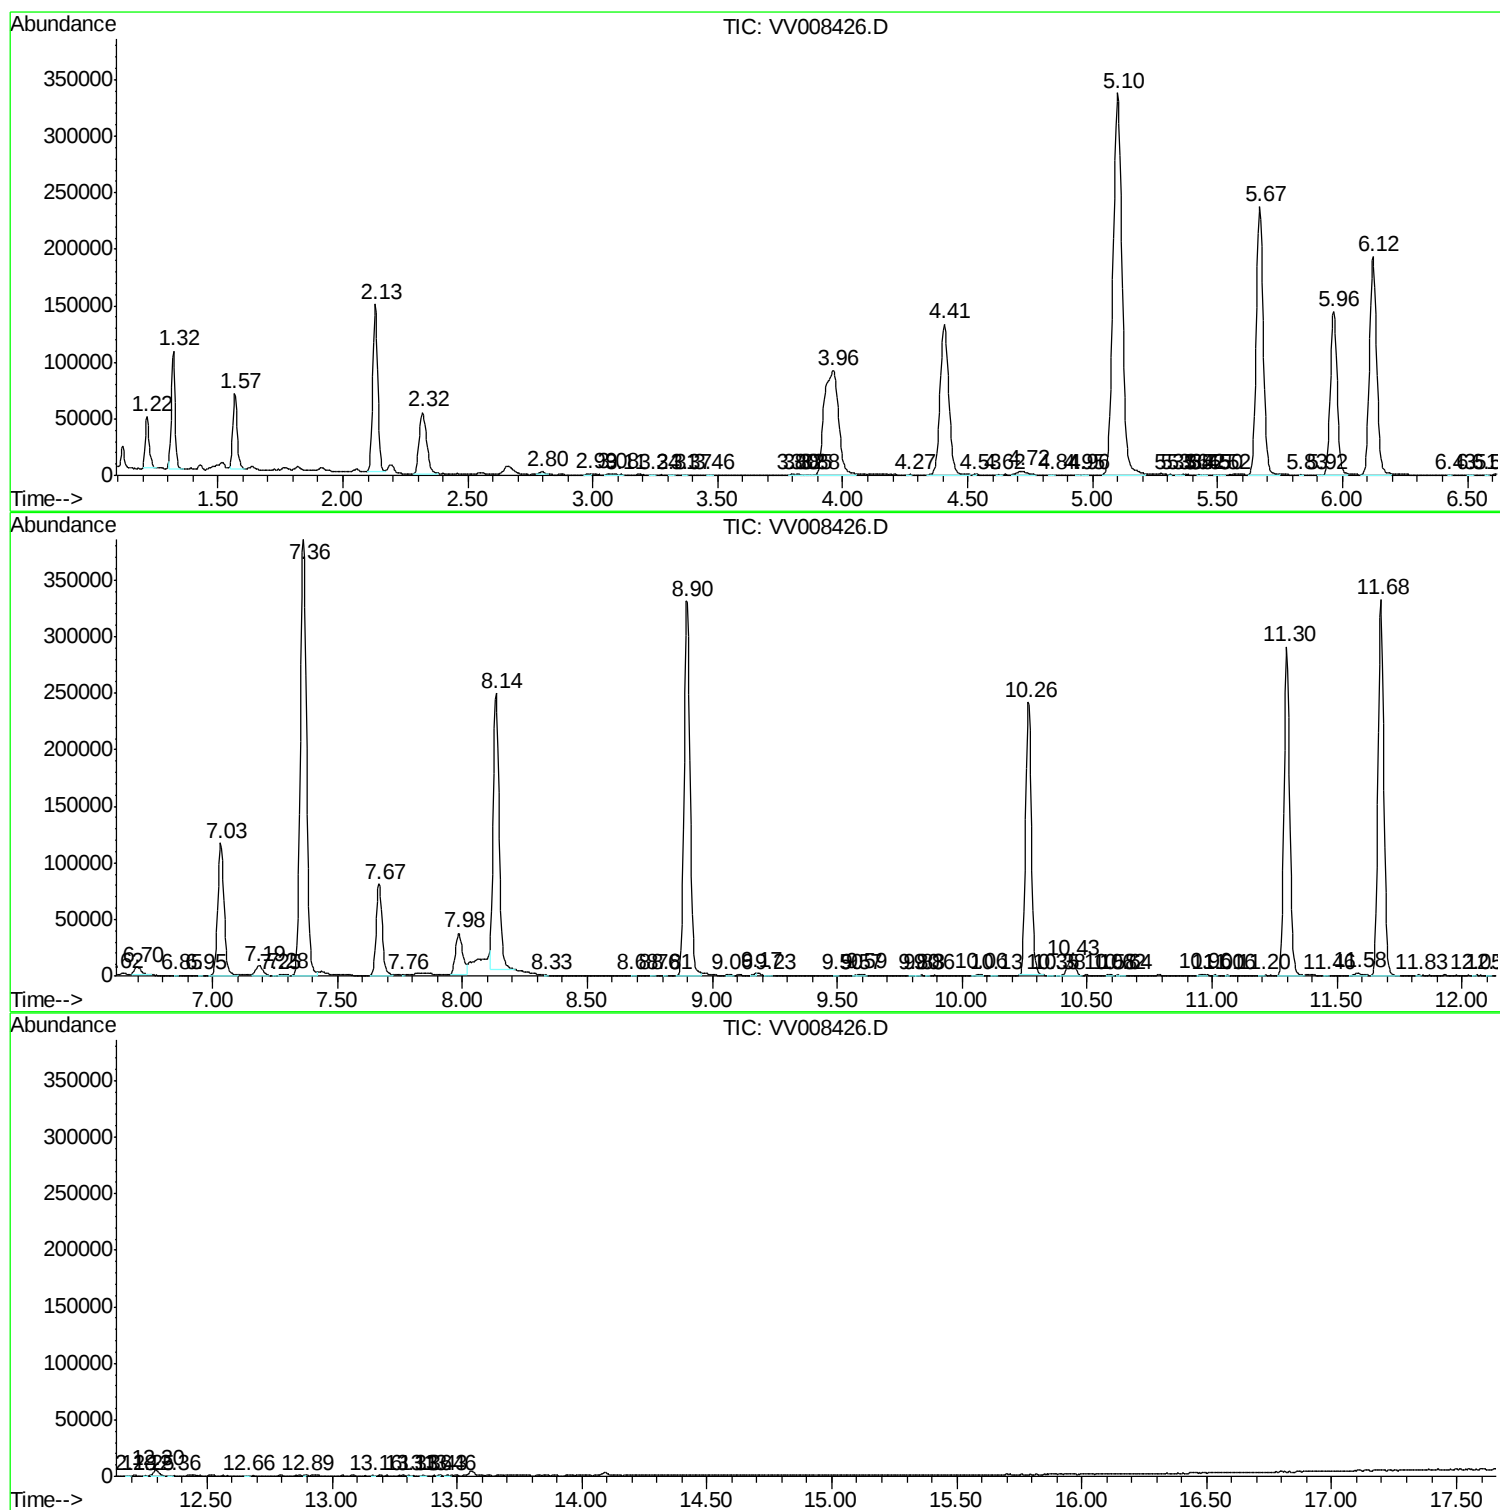

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102618\
Data File : VV008426.D
Acq On : 26 Oct 2018 12:30
Operator : SY/MD
Sample : J5670-02
Misc : 5.0 mL/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBP3










Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.32	12.15 ug/L	112400	1,4-Difluorobenzene	5.67

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Isopropyl Alcohol	60	C3H8O	000067-63-0	83
2		Isopropyl Alcohol	60	C3H8O	000067-63-0	83
3		Isopropyl Alcohol	60	C3H8O	000067-63-0	83
4		Propane, 2-ethoxy-	88	C5H12O	000625-54-7	43
5		R-(-)-1,2-propanediol	76	C3H8O2	004254-14-2	9

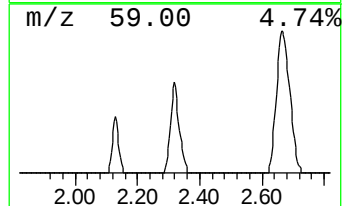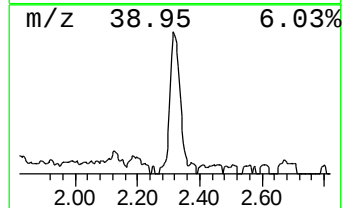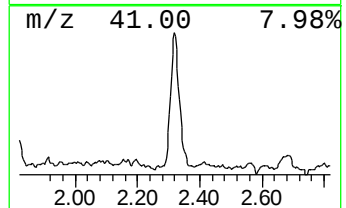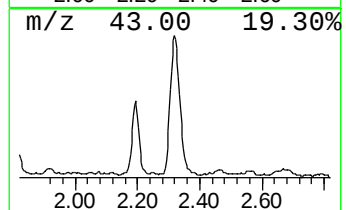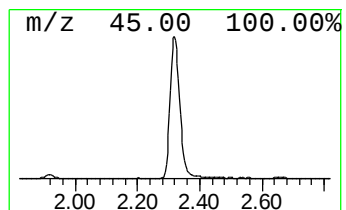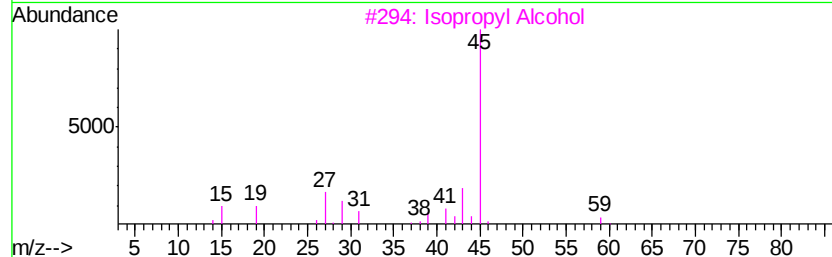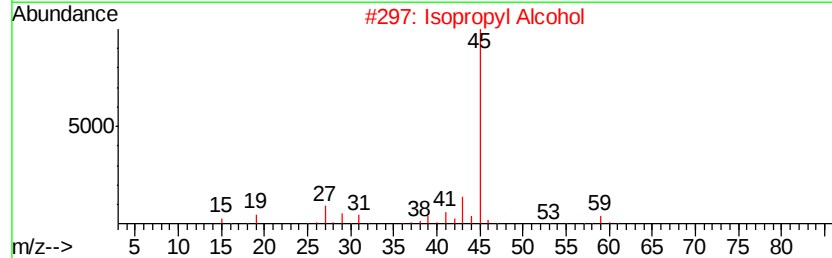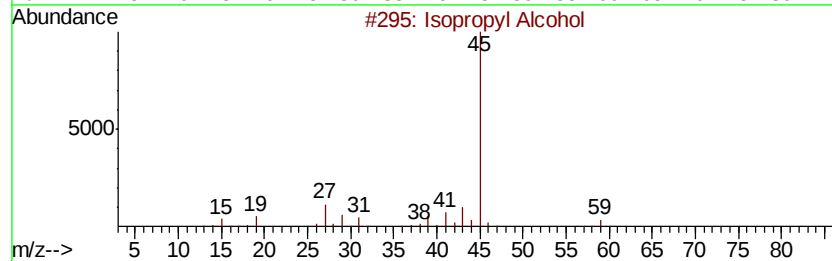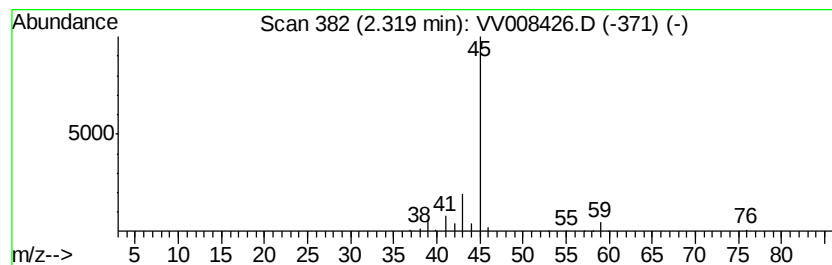

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102618\
Data File : VV008426.D
Acq On : 26 Oct 2018 12:30
Operator : SY/MD
Sample : J5670-02
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETBP3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.32	12.2	ug/L	112400	1	5.67	462588	50.0