


Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102618\
 Data File : VV008421.D
 Acq On : 26 Oct 2018 09:53
 Operator : SY/MD
 Sample : BFB51
 Misc : 5.0 mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB51

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102318WMA.M
 Title : VOC Analysis
 Last Update : Sat Oct 27 04:42:32 2018

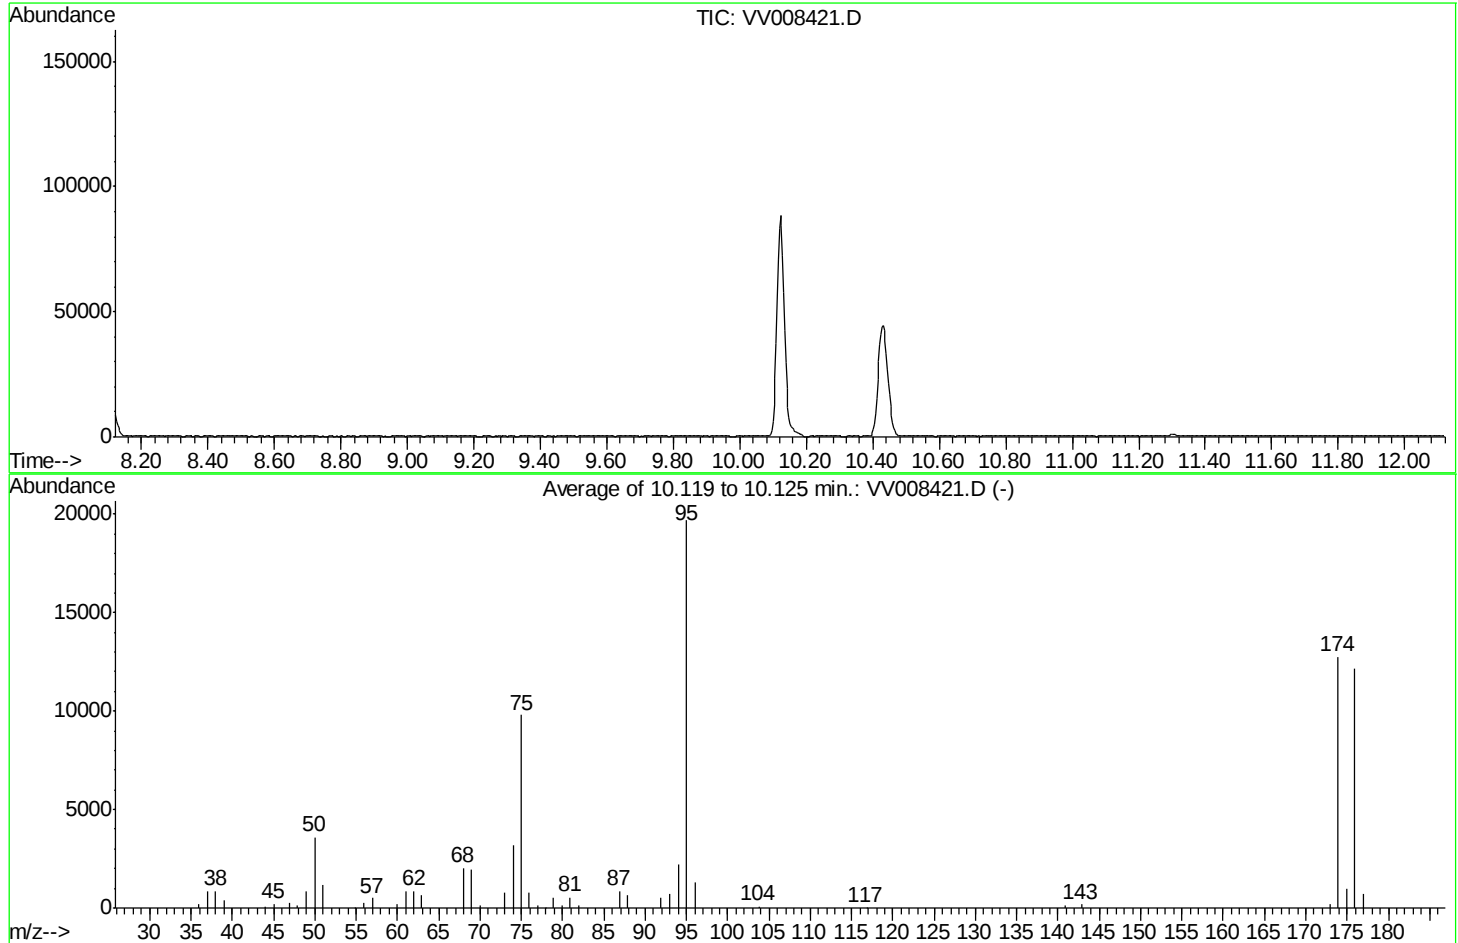

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	3607	PASS
75	95	30	80	49.8	9811	PASS
95	95	100	100	100.0	19688	PASS
96	95	5	9	6.7	1323	PASS
173	174	0.00	2	1.4	174	PASS
174	95	50	120	64.8	12755	PASS
175	174	5	9	7.6	970	PASS
176	174	95	101	95.2	12149	PASS
177	176	5	9	6.1	747	PASS

Scan 2797 (10.084 min): VV008421.D
BFB51

m/z	Abundance
39.90	141.0
43.90	260.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.90	181.0
36.90	821.0
38.00	863.0
39.00	372.0
44.00	354.0
45.00	219.0
46.90	251.0
47.80	162.0
49.00	843.0
50.00	3649.0
51.00	1134.0
55.90	286.0
57.00	491.0
60.00	183.0
61.00	819.0
62.00	858.0
62.90	649.0
68.00	1884.0
69.00	1970.0
69.90	157.0
73.00	745.0
74.00	3114.0
75.00	9558.0
75.90	767.0
77.00	149.0
77.90	101.0
78.90	505.0
79.90	140.0
80.90	547.0
81.90	114.0
86.90	805.0
87.90	716.0
91.90	515.0
93.00	758.0
94.00	2048.0
95.00	19568.0
96.00	1343.0
140.90	183.0
142.80	157.0
173.00	182.0
173.90	12125.0
174.90	885.0
175.90	11684.0
176.90	737.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.90	187.0
37.00	891.0
38.00	894.0
39.00	392.0
44.00	327.0
45.00	204.0
46.90	268.0
47.80	164.0
49.00	872.0
50.00	3745.0
51.00	1213.0
54.90	103.0
56.00	308.0
57.00	503.0
59.90	200.0
61.00	866.0
62.00	898.0
62.90	671.0
68.00	2110.0
69.00	2058.0
70.00	153.0
73.00	788.0
74.00	3225.0
75.00	10152.0
75.90	785.0
77.00	146.0
78.90	580.0
79.90	126.0
80.90	569.0
81.90	127.0
86.90	883.0
87.90	694.0
91.90	510.0
93.00	780.0
94.00	2278.0
95.00	20312.0
96.00	1367.0
103.80	113.0
140.90	169.0
142.80	188.0
173.00	180.0
173.90	13238.0
174.90	1008.0
175.90	12608.0
176.90	768.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51

m/z	Abundance
35.90	160.0
36.90	870.0
38.00	834.0
39.00	348.0
44.00	314.0
45.00	173.0
47.00	259.0
47.80	141.0
49.00	811.0
50.00	3427.0
51.00	1161.0
56.00	288.0
57.00	496.0
59.90	211.0
61.00	804.0
62.00	844.0
63.00	651.0
68.00	2085.0
69.00	1906.0
70.00	145.0
73.00	792.0
74.00	3166.0
75.00	9725.0
76.00	745.0
77.00	121.0
78.90	549.0
79.90	130.0
80.90	540.0
81.90	121.0
86.90	851.0
87.90	599.0
91.90	488.0
92.90	687.0
94.00	2231.0
95.00	19184.0
96.00	1259.0
103.80	104.0
116.80	100.0
140.80	133.0
142.80	191.0
173.00	161.0
173.90	12904.0
174.90	1017.0
175.90	12155.0
176.90	737.0

Instrument :
MSVOA_V
ClientSampleId :
BFB51