


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV102619\
 Data File : VV013366.D
 Acq On : 26 Oct 2019 09:53
 Operator : SY/MD
 Sample : BFB49
 Misc : 25.0ML/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB49

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR102119WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Tue Nov 05 07:35:33 2019

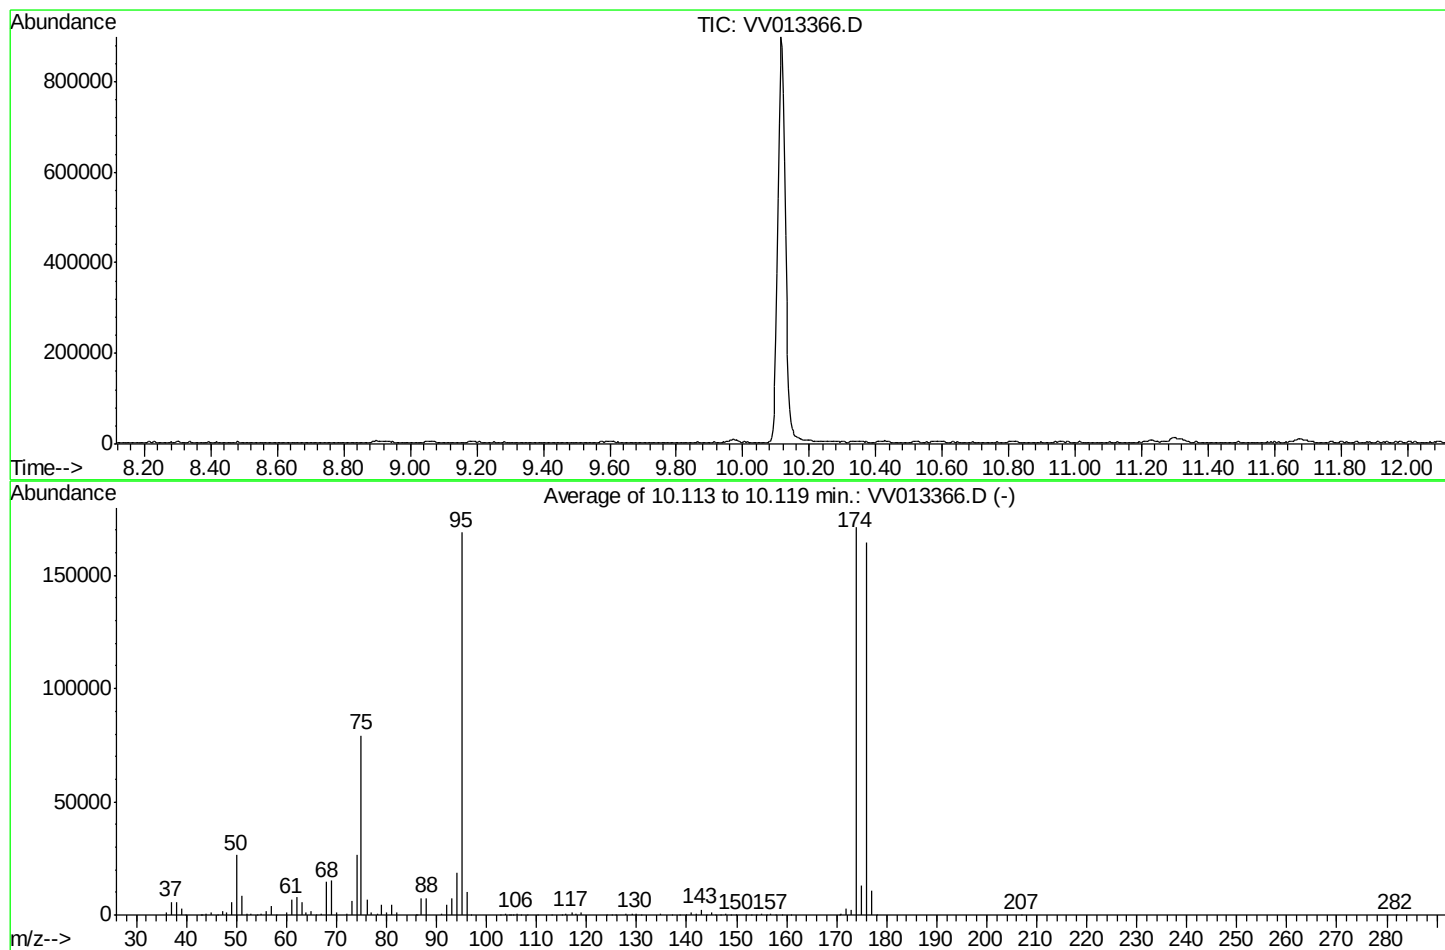

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.7	26557	PASS
75	95	30	80	47.0	79381	PASS
95	95	100	100	100.0	169002	PASS
96	95	5	9	6.1	10379	PASS
173	174	0.00	2	1.3	2299	PASS
174	95	50	120	101.3	171200	PASS
175	174	5	9	7.6	12966	PASS
176	174	95	101	96.2	164716	PASS
177	176	5	9	6.5	10706	PASS

m/z	Abundance
36.00	1130.0
37.00	5860.0
38.00	5681.0
39.00	2642.0
40.00	1290.0
41.00	125.0
43.10	211.0
44.00	1443.0
45.00	1209.0
46.20	235.0
47.10	1980.0
48.10	1185.0
49.00	5635.0
50.00	27232.0
51.00	8663.0
52.00	538.0
53.00	355.0
54.10	125.0
55.00	445.0
56.00	1866.0
57.00	3943.0
58.00	218.0
60.00	1246.0
61.00	7219.0
62.00	8044.0
63.00	6155.0
64.00	1333.0
65.00	1731.0
65.90	205.0
67.00	732.0
68.00	14868.0
69.00	15562.0
70.00	1156.0
72.00	803.0
73.00	6719.0
74.00	27760.0
75.00	81912.0
76.10	7130.0
76.90	1420.0
78.10	792.0
78.90	4753.0
79.90	1353.0
80.90	4745.0
81.90	1062.0
85.90	267.0
86.10	232.0
86.90	7395.0
87.90	7651.0
91.00	735.0
92.00	4626.0
93.00	7360.0
94.00	19656.0
95.00	174208.0
96.00	10583.0
97.00	252.0
102.80	126.0
103.90	658.0
104.70	184.0
106.00	737.0
106.80	186.0
108.00	150.0
112.90	127.0
114.90	245.0
115.90	733.0
117.00	1326.0
117.80	506.0
118.80	1101.0
123.90	122.0
125.10	163.0
125.80	109.0
127.90	581.0
129.10	479.0
129.90	676.0
130.90	286.0
134.90	449.0
137.10	198.0
139.90	172.0
141.00	1485.0
141.80	346.0
142.90	2622.0
144.00	152.0
144.90	1270.0
145.80	292.0
146.90	172.0
147.80	605.0
148.90	175.0
149.90	204.0
151.90	150.0
152.80	142.0
153.80	170.0
155.00	327.0
156.10	100.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

156.80	453.0
159.00	205.0
160.90	171.0
170.90	469.0
172.00	2688.0
172.90	2358.0
173.90	177408.0
175.00	13592.0
175.90	170304.0
177.00	11028.0
178.00	240.0
207.00	269.0
281.90	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	1160.0
37.00	5702.0
38.00	5501.0
39.00	2712.0
39.90	1244.0
41.00	145.0
43.20	228.0
44.00	1442.0
45.00	1124.0
46.30	231.0
47.10	1812.0
48.10	965.0
49.00	5465.0
50.00	26336.0
51.00	8256.0
52.00	599.0
53.00	425.0
54.10	103.0
55.10	359.0
56.00	1704.0
57.10	3716.0
57.90	214.0
59.90	1125.0
61.00	7004.0
62.00	7281.0
63.00	5774.0
64.00	1188.0
65.00	1453.0
66.00	211.0
67.00	713.0
68.00	13892.0
69.00	14702.0
70.00	942.0
72.00	644.0
73.00	6435.0
74.00	25784.0
75.00	77392.0
76.10	6497.0
76.90	1327.0
78.20	718.0
78.90	4455.0
79.90	1456.0
80.90	4567.0
81.90	993.0
85.80	208.0
86.90	7582.0
87.90	7617.0
91.00	559.0
92.00	4500.0
93.00	6788.0
94.00	17832.0
95.00	164992.0
96.00	10236.0
97.00	227.0
103.90	635.0
104.60	221.0
105.20	112.0
106.00	659.0
106.80	119.0
108.00	122.0
112.90	148.0
115.00	241.0
115.90	672.0
117.00	1309.0
117.90	460.0
118.90	1033.0
123.90	126.0
125.00	114.0
127.90	486.0
129.10	435.0
129.90	684.0
130.90	256.0
134.80	444.0
137.00	180.0
139.90	144.0
141.00	1493.0
141.80	215.0
142.90	2405.0
144.90	1171.0
145.80	264.0
146.80	116.0
147.90	615.0
148.90	217.0
150.00	184.0
151.90	134.0
152.80	143.0
153.90	108.0
155.10	363.0
156.00	111.0
156.80	426.0
159.00	168.0
161.00	214.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

171.00	489.0
171.90	2507.0
172.90	2400.0
173.90	161536.0
175.00	12091.0
175.90	155008.0
177.00	10034.0
178.10	230.0
207.00	197.0
281.90	150.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

Scan 2792 (10.068 min): VV013366.D
BFB49

m/z	Abundance
39.90	986.0
41.00	153.0
41.80	153.0
44.00	1114.0
46.10	111.0
63.90	101.0
77.20	128.0
77.90	135.0
101.80	107.0
118.00	106.0
130.50	105.0
133.70	126.0
175.90	105.0
207.20	128.0
281.00	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	1002.0
37.00	5896.0
38.00	5363.0
39.00	2488.0
40.00	1332.0
42.90	191.0
43.90	1436.0
45.00	1217.0
46.00	221.0
47.20	1982.0
48.00	1127.0
49.00	5391.0
50.00	26104.0
51.00	8374.0
52.00	414.0
52.90	272.0
54.00	140.0
54.90	569.0
56.00	1796.0
57.00	3711.0
58.10	238.0
60.00	1298.0
61.00	6847.0
62.00	7675.0
63.00	5847.0
64.00	1363.0
65.00	1756.0
65.90	173.0
67.00	583.0
68.00	14776.0
69.00	15065.0
70.00	1265.0
72.00	864.0
73.10	6387.0
74.00	26632.0
75.00	78840.0
76.10	7265.0
77.00	1190.0
78.10	762.0
78.90	4684.0
80.00	1188.0
80.90	4568.0
82.00	955.0
85.80	315.0
87.00	6739.0
88.00	7176.0
91.00	764.0
92.00	4283.0
93.00	7179.0
94.00	19192.0
95.00	167808.0
96.00	10320.0
97.00	339.0
102.80	123.0
103.90	628.0
104.90	165.0
106.00	744.0
106.80	196.0
108.10	155.0
110.10	107.0
112.90	111.0
114.90	257.0
115.90	705.0
117.00	1299.0
117.90	522.0
118.80	1098.0
125.10	179.0
125.80	149.0
128.00	592.0
129.10	437.0
129.80	718.0
130.80	324.0
133.90	126.0
134.90	406.0
137.10	237.0
138.70	122.0
139.90	152.0
141.00	1288.0
141.90	408.0
142.90	2618.0
144.00	177.0
144.90	1199.0
145.80	332.0
147.00	227.0
147.80	462.0
148.80	169.0
149.80	170.0
151.90	136.0
152.80	137.0
153.80	210.0
154.90	308.0
156.80	402.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

157.80	112.0
159.10	182.0
160.80	130.0
170.70	419.0
172.00	2568.0
172.90	2139.0
173.90	174656.0
175.00	13216.0
175.90	169152.0
177.00	11057.0
177.90	238.0
207.00	267.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49