

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102620\
 Data File : VV019110.D
 Acq On : 26 Oct 2020 11:19
 Operator : SY/MD
 Sample : VV1026WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK98

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	81	rVB	165106	159655	13.75%	1.798%
2	1.579	145	152	165	rVB	137122	152477	13.13%	1.717%
3	2.123	311	321	351	rVB	270683	417414	35.94%	4.701%
4	2.405	407	409	414	rVB3	703	383	0.03%	0.004%
5	2.528	442	447	459	rVB5	1357	1916	0.16%	0.022%
6	2.910	565	566	569	rVB2	327	116	0.01%	0.001%
7	3.013	595	598	600	rBV	255	158	0.01%	0.002%
8	3.026	600	602	606	rVV2	256	164	0.01%	0.002%
9	3.065	613	614	617	rBV2	232	112	0.01%	0.001%
10	3.190	650	653	658	rBV2	211	192	0.02%	0.002%
11	3.492	744	747	751	rVB	430	351	0.03%	0.004%
12	3.511	751	753	754	rBV	141	56	0.00%	0.001%
13	3.566	766	770	771	rBV2	203	128	0.01%	0.001%
14	3.833	851	853	855	rBV2	214	98	0.01%	0.001%
15	3.910	867	877	913	rBV	87065	253990	21.87%	2.860%
16	4.373	1005	1021	1047	rBV	191472	471550	40.60%	5.310%
17	4.737	1129	1134	1137	rBV2	231	247	0.02%	0.003%
18	4.872	1171	1176	1180	rBV2	433	490	0.04%	0.006%
19	5.071	1221	1238	1273	rBV2	454540	1161467	100.00%	13.080%
20	5.508	1371	1374	1376	rBV2	307	203	0.02%	0.002%
21	5.640	1403	1415	1443	rBV	345239	693036	59.67%	7.805%
22	5.936	1498	1507	1519	rVB5	3019	6077	0.52%	0.068%
23	6.093	1542	1556	1585	rBV	264036	537785	46.30%	6.056%
24	6.389	1645	1648	1650	rBV2	450	252	0.02%	0.003%
25	6.444	1664	1665	1667	rBV2	202	64	0.01%	0.001%
26	6.553	1696	1699	1701	rBV	220	141	0.01%	0.002%
27	6.672	1734	1736	1739	rBV2	402	180	0.02%	0.002%
28	6.791	1772	1773	1774	rBV2	119	38	0.00%	0.000%
29	6.820	1780	1782	1785	rVB	310	108	0.01%	0.001%
30	6.881	1799	1801	1804	rBV2	180	100	0.01%	0.001%
31	7.007	1829	1840	1857	rBV	146574	263952	22.73%	2.973%
32	7.289	1926	1928	1931	rBV2	328	152	0.01%	0.002%
33	7.338	1931	1943	1967	rBV	518962	882638	75.99%	9.940%
34	7.643	2027	2038	2068	rBV	108310	192475	16.57%	2.168%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102620\
 Data File : VV019110.D
 Acq On : 26 Oct 2020 11:19
 Operator : SY/MD
 Sample : VV1026WBL01
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK98

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	7.846	2099	2101	2102	rBV	343	136	0.01%	0.002%
36	7.933	2126	2128	2132	rBV2	267	182	0.02%	0.002%
37	8.039	2158	2161	2162	rBV	261	129	0.01%	0.001%
38	8.106	2171	2182	2206	rBV	335767	565706	48.71%	6.371%
39	8.418	2278	2279	2280	rBV	342	116	0.01%	0.001%
40	8.531	2311	2314	2317	rBV2	473	283	0.02%	0.003%
41	8.627	2342	2344	2346	rBV2	561	261	0.02%	0.003%
42	8.678	2353	2360	2364	rBV2	491	606	0.05%	0.007%
43	8.871	2409	2420	2454	rBV	541423	876673	75.48%	9.873%
44	9.180	2511	2516	2519	rBV	316	378	0.03%	0.004%
45	9.244	2534	2536	2541	rBV2	306	298	0.03%	0.003%
46	9.293	2549	2551	2554	rBV	412	177	0.02%	0.002%
47	9.460	2599	2603	2610	rBV2	436	639	0.06%	0.007%
48	9.785	2700	2704	2710	rVB3	322	314	0.03%	0.004%
49	10.061	2787	2790	2794	rVB	345	240	0.02%	0.003%
50	10.238	2830	2845	2864	rBV	352789	553776	47.68%	6.236%
51	10.460	2910	2914	2916	rBV2	458	406	0.03%	0.005%
52	10.894	3044	3049	3054	rBV2	324	349	0.03%	0.004%
53	10.952	3063	3067	3068	rBV2	413	230	0.02%	0.003%
54	11.270	3155	3166	3188	rBV	529651	819338	70.54%	9.227%
55	11.463	3223	3226	3229	rBV2	440	351	0.03%	0.004%
56	11.646	3271	3283	3302	rBV	549467	860570	74.09%	9.691%
57	13.366	3816	3818	3821	rBV2	452	262	0.02%	0.003%
58	13.463	3846	3848	3849	rBV	272	69	0.01%	0.001%


Sum of corrected areas: 8879654

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102620\
Data File : VV019110.D
Acq On : 26 Oct 2020 11:19
Operator : SY/MD
Sample : VV1026WBL01
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK98

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

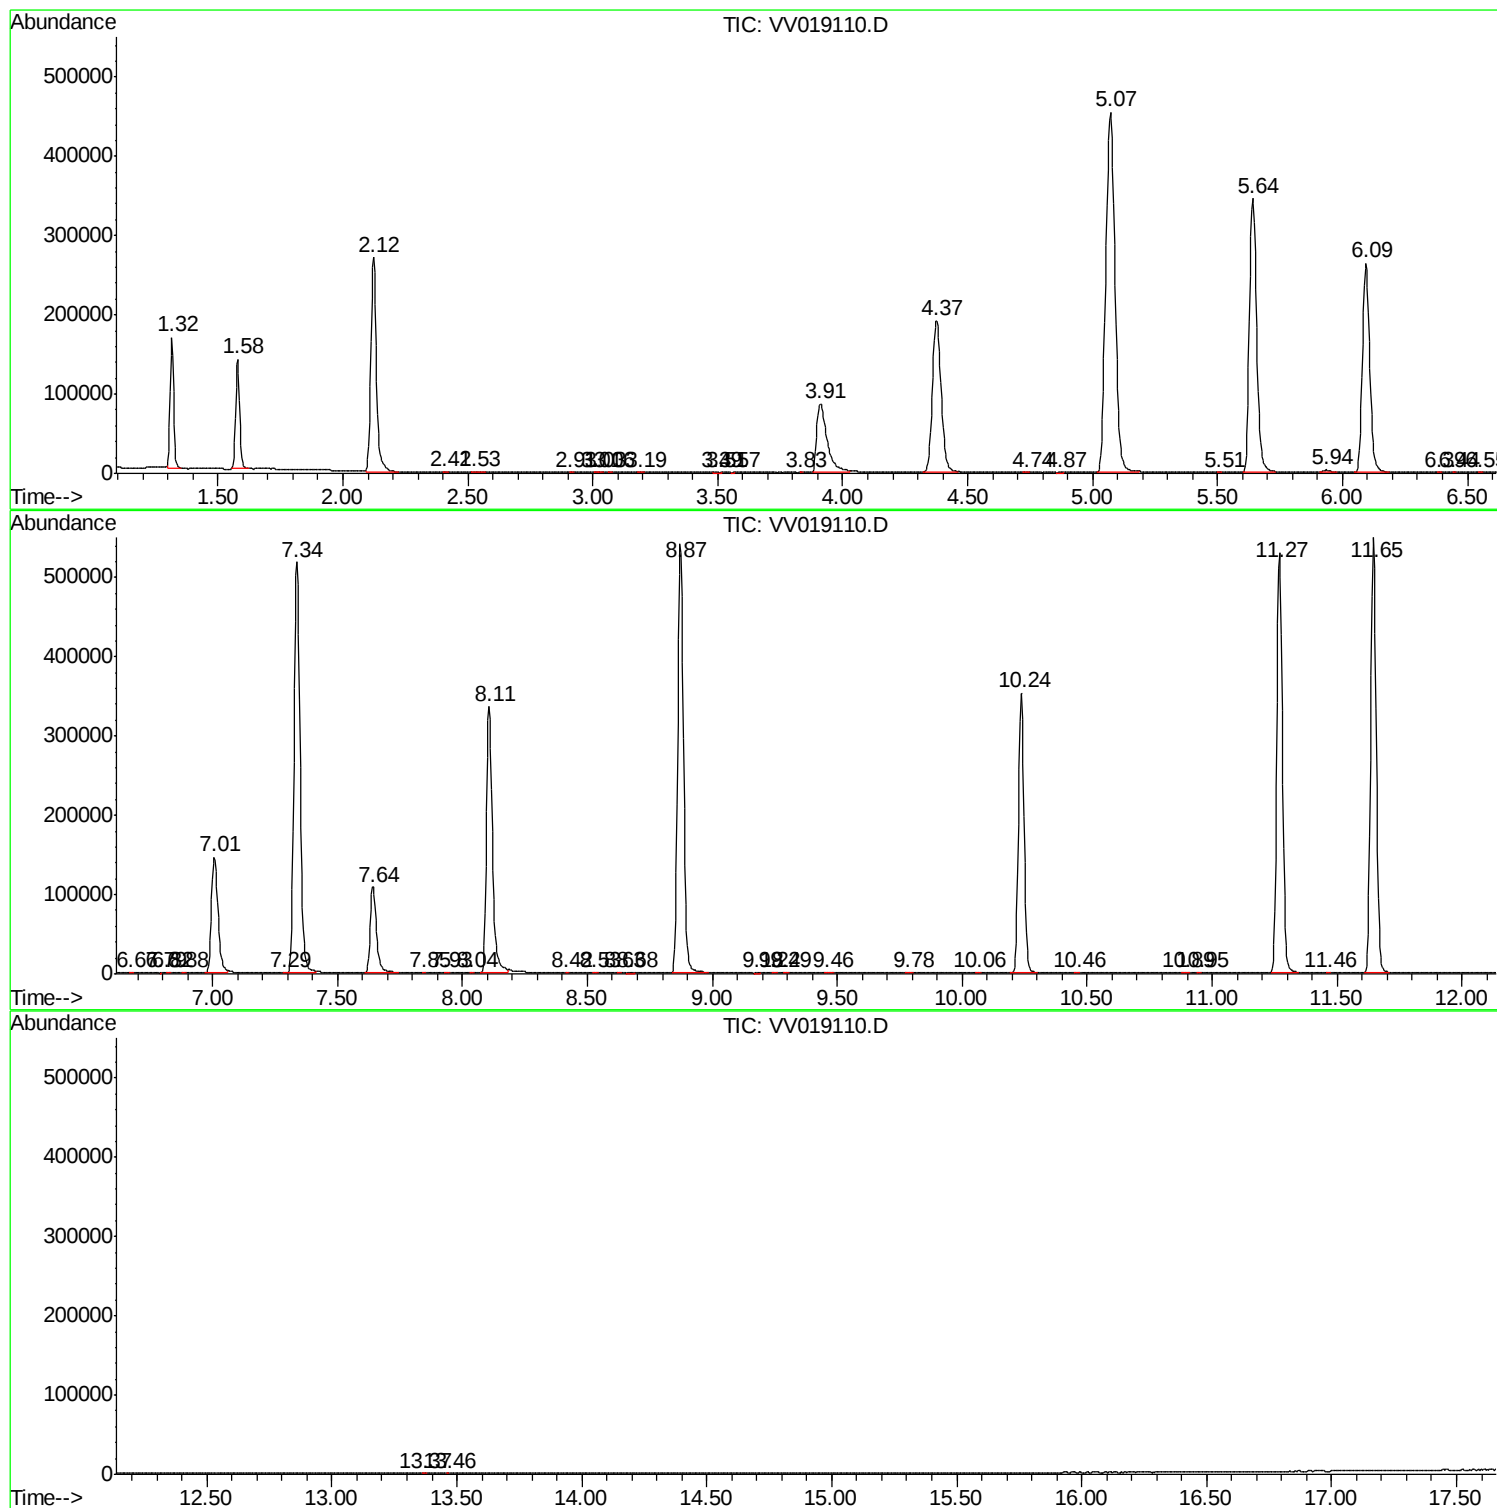

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102620\
Data File : VV019110.D
Acq On : 26 Oct 2020 11:19
Operator : SY/MD
Sample : VV1026WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK98

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_V\DATA\VV102620\
Data File : VV019110.D
Acq On : 26 Oct 2020 11:19
Operator : SY/MD
Sample : VV1026WBL01
Misc : 5.0mL/MSV0A_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSV0A_V
ClientSampleId :
VBLK98

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc