

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102620\
 Data File : VV019121.D
 Acq On : 26 Oct 2020 15:56
 Operator : SY/MD
 Sample : VIBLK71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.315	64	70	84	rVB	158379	154832	13.71%	1.802%
2	1.576	145	151	166	rVB	134268	154642	13.70%	1.800%
3	2.122	310	321	351	rVB	266717	411492	36.44%	4.789%
4	2.521	439	445	454	rVB4	1194	1665	0.15%	0.019%
5	2.621	473	476	479	rBV2	267	181	0.02%	0.002%
6	2.663	487	489	490	rBV	240	101	0.01%	0.001%
7	2.843	542	545	547	rBV	173	132	0.01%	0.002%
8	2.910	564	566	567	rBV	148	47	0.00%	0.001%
9	2.968	582	584	587	rVB	256	104	0.01%	0.001%
10	3.145	633	639	641	rBV	507	505	0.04%	0.006%
11	3.341	696	700	704	rBV	272	259	0.02%	0.003%
12	3.364	704	707	709	rVV2	142	77	0.01%	0.001%
13	3.412	719	722	727	rBV2	238	185	0.02%	0.002%
14	3.434	727	729	732	rVV	156	59	0.01%	0.001%
15	3.489	743	746	751	rVB2	262	229	0.02%	0.003%
16	3.515	751	754	756	rBV	136	101	0.01%	0.001%
17	3.566	768	770	776	rVB	274	163	0.01%	0.002%
18	3.634	789	791	795	rVB2	263	155	0.01%	0.002%
19	3.659	796	799	803	rBV2	244	152	0.01%	0.002%
20	3.691	807	809	810	rBV	132	33	0.00%	0.000%
21	3.765	829	832	834	rBV	280	182	0.02%	0.002%
22	3.791	838	840	841	rBV	176	60	0.01%	0.001%
23	3.827	849	851	852	rBV	196	65	0.01%	0.001%
24	3.907	865	876	904	rBV	84313	235100	20.82%	2.736%
25	4.376	1007	1022	1047	rBV	184679	445584	39.46%	5.186%
26	4.662	1109	1111	1112	rBV	170	84	0.01%	0.001%
27	4.791	1147	1151	1154	rBV3	331	324	0.03%	0.004%
28	4.884	1177	1180	1185	rBV2	304	313	0.03%	0.004%
29	4.971	1204	1207	1208	rBV	160	78	0.01%	0.001%
30	5.071	1221	1238	1264	rBV2	443297	1129084	100.00%	13.140%
31	5.354	1319	1326	1329	rBV2	436	510	0.05%	0.006%
32	5.383	1333	1335	1336	rBV	232	93	0.01%	0.001%
33	5.412	1341	1344	1346	rBV	251	187	0.02%	0.002%
34	5.473	1361	1363	1365	rBV2	230	81	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102620\
 Data File : VV019121.D
 Acq On : 26 Oct 2020 15:56
 Operator : SY/MD
 Sample : VIBLK71
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
 Title : VOC Analysis

35	5.486	1365	1367	1371	rVB	388	185	0.02%	0.002%
36	5.515	1371	1376	1377	rBV3	298	191	0.02%	0.002%
37	5.640	1403	1415	1448	rBV	335865	676036	59.87%	7.867%
38	5.933	1495	1506	1521	rVB6	3223	7236	0.64%	0.084%
39	5.990	1522	1524	1528	rVB2	329	173	0.02%	0.002%
40	6.048	1539	1542	1543	rBV	306	160	0.01%	0.002%
41	6.093	1543	1556	1579	rVV	261456	517615	45.84%	6.024%
42	6.267	1607	1610	1613	rBV3	517	342	0.03%	0.004%
43	6.408	1651	1654	1659	rBV	255	236	0.02%	0.003%
44	6.428	1659	1660	1664	rVV2	186	117	0.01%	0.001%
45	6.701	1741	1745	1749	rBV3	415	384	0.03%	0.004%
46	6.724	1749	1752	1753	rBV	237	136	0.01%	0.002%
47	6.804	1775	1777	1780	rBV2	215	133	0.01%	0.002%
48	6.849	1788	1791	1794	rVB2	291	194	0.02%	0.002%
49	6.875	1794	1799	1800	rBV2	185	141	0.01%	0.002%
50	6.891	1801	1804	1807	rVV	374	256	0.02%	0.003%
51	7.006	1827	1840	1869	rBV	139859	258364	22.88%	3.007%
52	7.293	1926	1929	1931	rBV2	356	234	0.02%	0.003%
53	7.338	1931	1943	1976	rVV	509717	876796	77.66%	10.204%
54	7.643	2028	2038	2057	rBV	102968	180289	15.97%	2.098%
55	7.884	2110	2113	2117	rBV	436	363	0.03%	0.004%
56	7.929	2123	2127	2130	rBV	354	266	0.02%	0.003%
57	8.000	2143	2149	2159	rVB5	2660	3388	0.30%	0.039%
58	8.048	2161	2164	2169	rVB2	468	425	0.04%	0.005%
59	8.106	2172	2182	2215	rBV	316605	538926	47.73%	6.272%
60	8.659	2352	2354	2356	rBV	267	135	0.01%	0.002%
61	8.675	2357	2359	2365	rVB3	392	322	0.03%	0.004%
62	8.704	2365	2368	2370	rBV2	302	221	0.02%	0.003%
63	8.768	2385	2388	2393	rVB	447	369	0.03%	0.004%
64	8.871	2408	2420	2452	rBV	526503	853782	75.62%	9.936%
65	9.045	2472	2474	2478	rBV	364	264	0.02%	0.003%
66	9.103	2487	2492	2496	rBV2	375	420	0.04%	0.005%
67	9.344	2564	2567	2569	rBV2	285	194	0.02%	0.002%
68	9.701	2674	2678	2679	rBV2	189	134	0.01%	0.002%
69	9.749	2690	2693	2696	rBV2	300	215	0.02%	0.003%
70	9.823	2714	2716	2720	rVB2	344	187	0.02%	0.002%
71	10.238	2833	2845	2865	rBV	333478	524296	46.44%	6.102%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV102620\
Data File : VV019121.D
Acq On : 26 Oct 2020 15:56
Operator : SY/MD
Sample : VIBLK71
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK71

Integration Parameters: LSCINT.P

Integrator: RTE
Smoothing : OFF
Sampling : 1
Start Thrs: 0.2
Stop Thrs : 0

Filtering: 5
Min Area: 0 % of largest Peak
Max Peaks: 100
Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Title : VOC Analysis

72	10.344	2875	2878	2883	rVB2	335	278	0.02%	0.003%
73	10.373	2883	2887	2890	rBV2	314	316	0.03%	0.004%
74	10.495	2921	2925	2927	rBV2	282	200	0.02%	0.002%
75	11.270	3155	3166	3188	rBV	520322	791295	70.08%	9.209%
76	11.646	3270	3283	3307	rBV	532304	820796	72.70%	9.552%


Sum of corrected areas: 8592869

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV102620\
Data File : VV019121.D
Acq On : 26 Oct 2020 15:56
Operator : SY/MD
Sample : VIBLK71
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
VIBLK71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

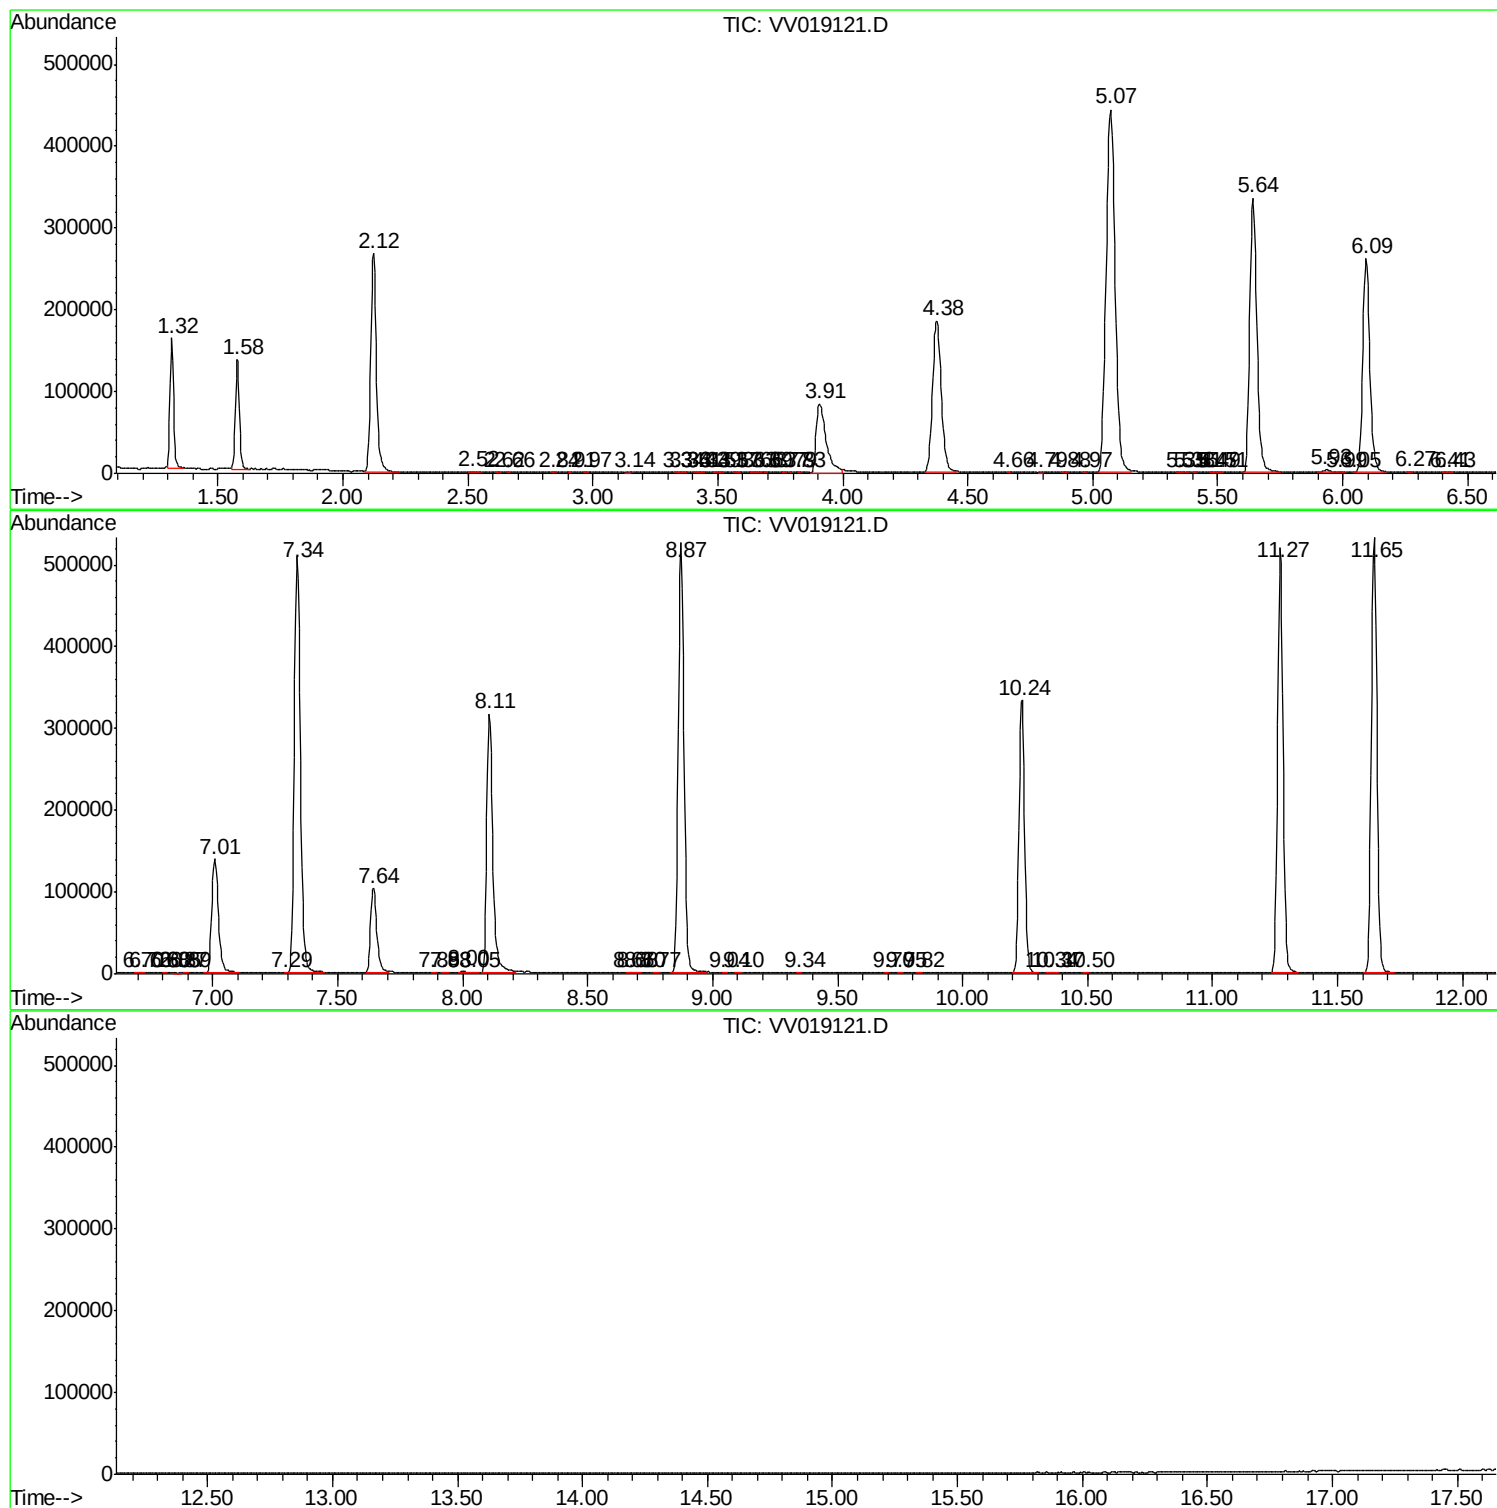

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102620\
Data File : VV019121.D
Acq On : 26 Oct 2020 15:56
Operator : SY/MD
Sample : VIBLK71
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV102620\
Data File : VV019121.D
Acq On : 26 Oct 2020 15:56
Operator : SY/MD
Sample : VIBLK71
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK71

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc