


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023048.D
Acq On : 26 Oct 2021 19:14
Operator : SY/MD
Sample : M4277-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1DL

Manual IntegrationsAPPROVED

Quant Time: Oct 27 01:35:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 27 01:29:33 2021
Response via : Initial Calibration

Reviewed By :John Carlone 10/27/2021
Supervised By :Mahesh Dadoda 10/27/2021

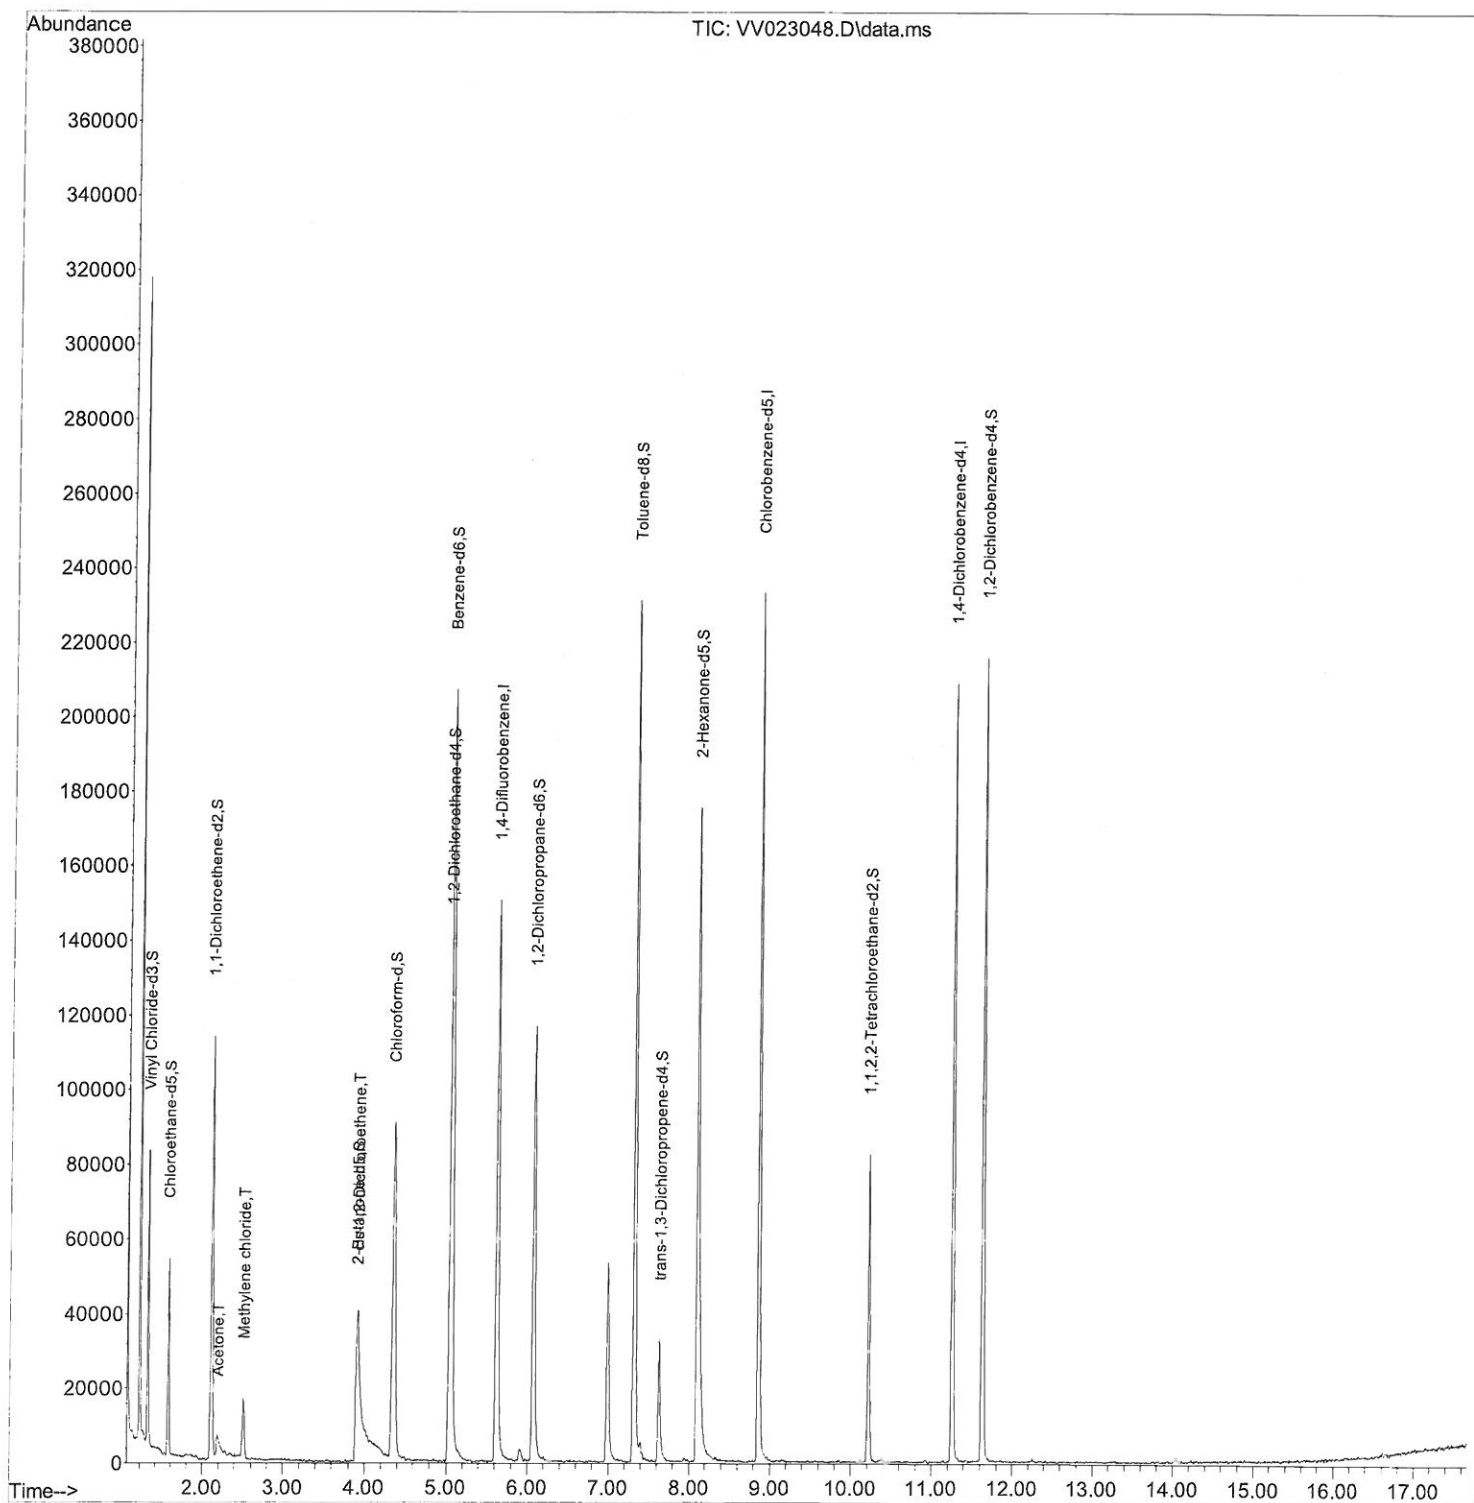

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023048.D
 Acq On : 26 Oct 2021 19:14
 Operator : SY/MD
 Sample : M4277-16DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE1DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/27/2021
 Supervised By :Mahesh Dadoda 10/27/2021

Quant Time: Oct 27 01:35:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 01:29:33 2021
 Response via : Initial Calibration

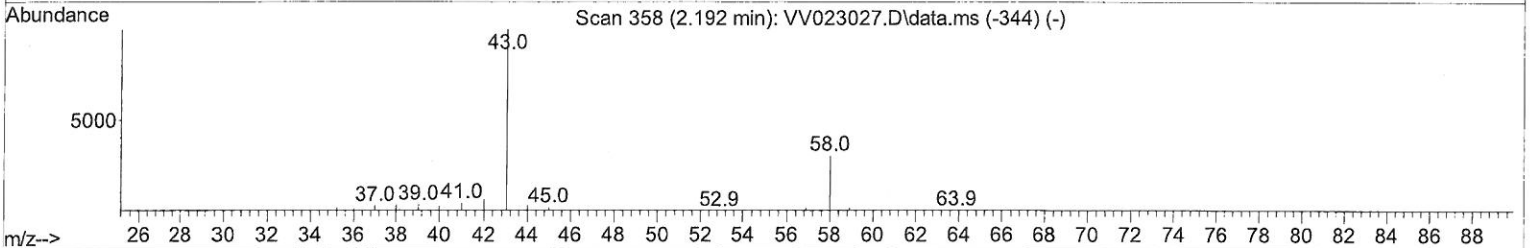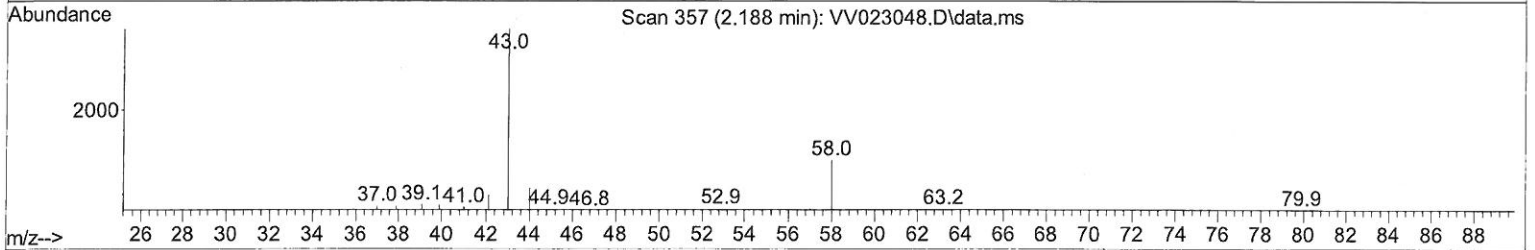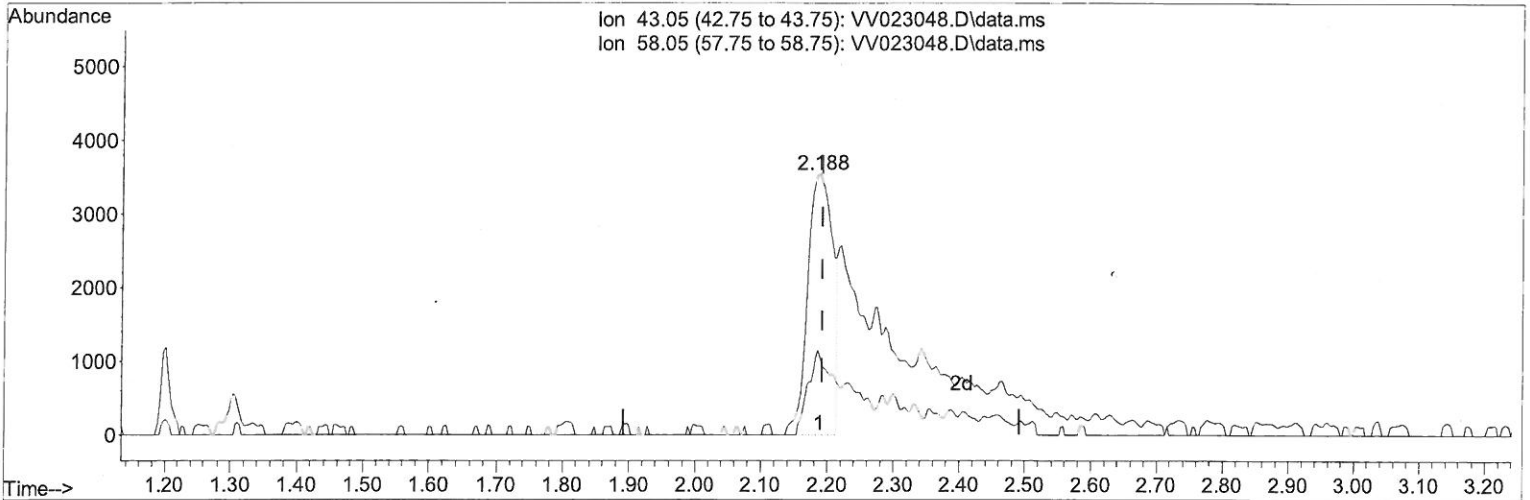

TIC: VV023048.D\data.ms

(13) Acetone (T)

2.188min (-0.003) 10.09 ug/L

response 9382

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	31.57
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023048.D
Acq On : 26 Oct 2021 19:14
Operator : SY/MD
Sample : M4277-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1DL

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/27/2021
Supervised By :Mahesh Dadoda 10/27/2021

Quant Time: Oct 27 01:36:38 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Oct 27 01:29:33 2021
Response via : Initial Calibration

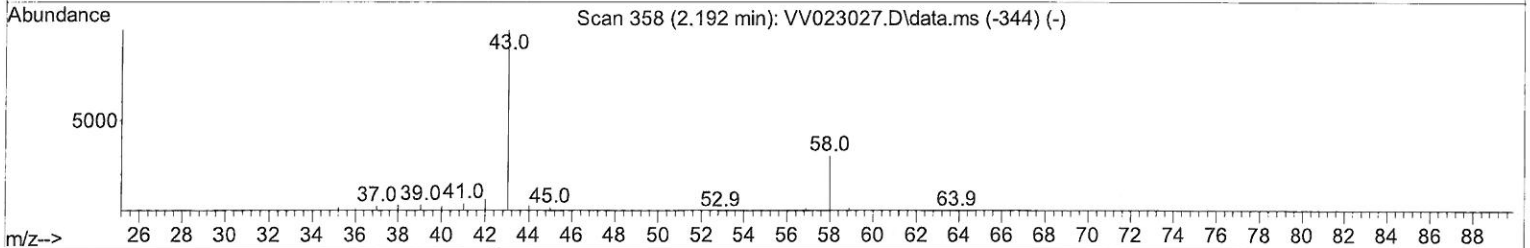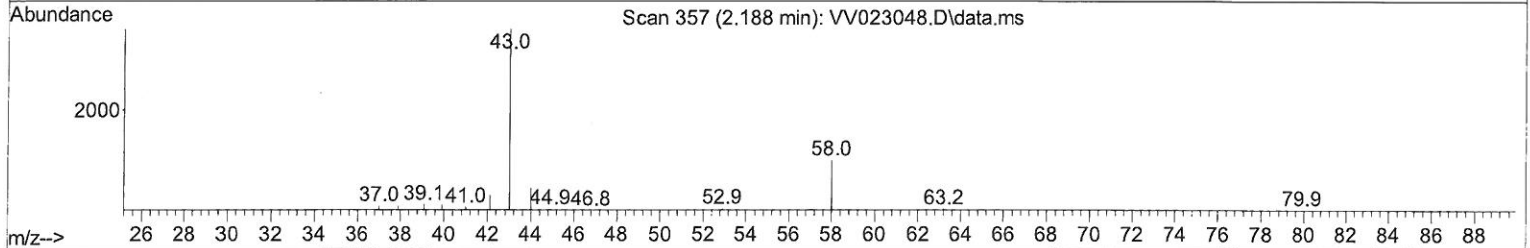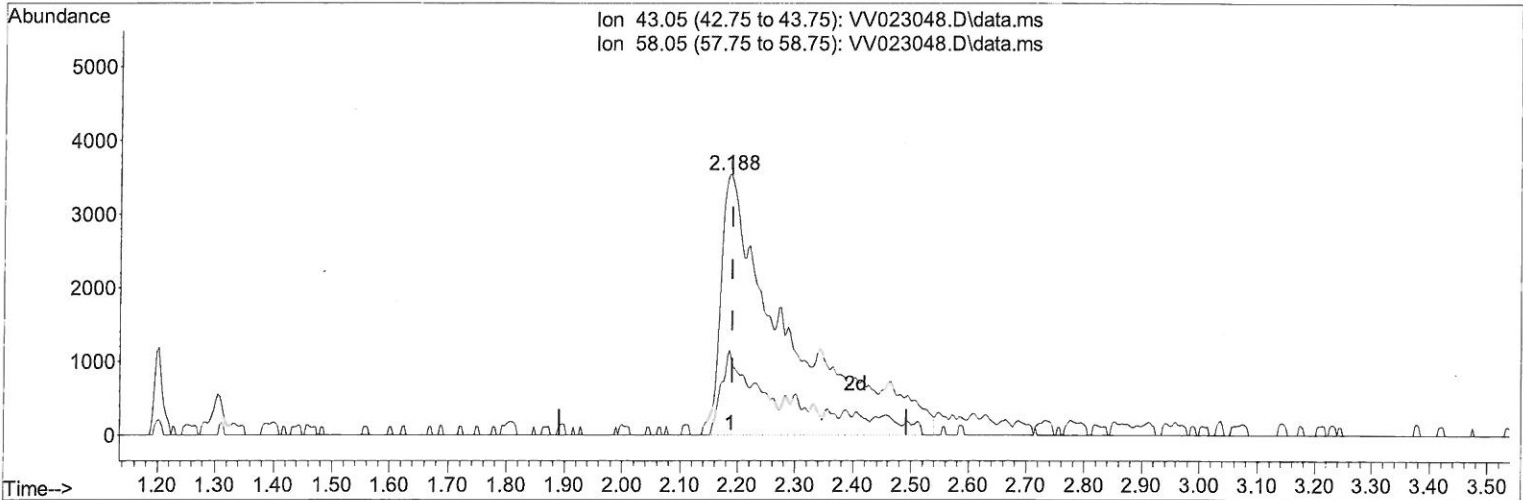

TIC: VV023048.D\data.ms

(13) Acetone (T)

2.188min (-0.003) 30.44 ug/L m

response 28293

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	10.47
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
11/02/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023048.D
 Acq On : 26 Oct 2021 19:14
 Operator : SY/MD
 Sample : M4277-16DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE1DL

Manual Integrations APPROVED

Reviewed By : John Carlone 10/27/2021
 Supervised By : Mahesh Dadoda 10/27/2021

Quant Time: Oct 27 01:35:38 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Oct 27 01:29:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	135154	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	133072	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57531	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	49697	4.208	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	84.200%		
7) Chloroethane-d5	1.568	69	32730	4.480	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	89.600%		
11) 1,1-Dichloroethene-d2	2.108	63	58515	3.435	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	68.600%		
20) 2-Butanone-d5	3.902	46	81411	42.972	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	85.940%		
24) Chloroform-d	4.349	84	96234	5.012	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	100.200%		
26) 1,2-Dichloroethane-d4	5.034	65	44703	4.939	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	98.800%		
32) Benzene-d6	5.050	84	189961	4.890	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	97.800%		
36) 1,2-Dichloropropane-d6	6.072	67	59393	4.966	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	99.400%		
41) Toluene-d8	7.317	98	158631	4.546	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	91.000%		
43) trans-1,3-Dichloroprop...	7.629	79	19766	4.717	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	94.400%		
46) 2-Hexanone-d5	8.092	63	73295	47.244	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	94.480%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39705	4.808	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	96.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	57747	5.626	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	112.600%		
Target Compounds						
13) Acetone	2.188	43	28293m	30.440	ug/L	Qvalue
16) Methylene chloride	2.507	84	6607	0.869	ug/L	97
22) cis-1,2-Dichloroethene	3.915	96	8311	0.992	ug/L #	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed