

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023028.D
 Acq On : 26 Oct 2021 10:39
 Operator : SY/MD
 Sample : VV1026WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	16	20	29	rVB3	4928	5155	1.33%	0.170%
2	1.240	59	62	72	rVB3	3298	4259	1.10%	0.141%
3	1.304	75	82	99	rVB	88429	91889	23.76%	3.035%
4	1.568	156	164	176	rVB	54844	62026	16.04%	2.049%
5	2.105	321	331	348	rBV	96561	133123	34.43%	4.397%
6	2.500	447	454	463	rBV5	3543	5651	1.46%	0.187%
7	3.915	877	894	907	rBV2	22643	75783	19.60%	2.503%
8	4.349	1013	1029	1055	rVB2	70992	180515	46.68%	5.963%
9	5.047	1230	1246	1274	rBV3	164615	386687	100.00%	12.772%
10	5.619	1412	1424	1453	rBV	115644	230886	59.71%	7.626%
11	5.908	1502	1514	1530	rVB5	5041	9797	2.53%	0.324%
12	6.072	1552	1565	1586	rBV	85505	172527	44.62%	5.699%
13	6.992	1837	1851	1876	rBV	39762	76213	19.71%	2.517%
14	7.150	1891	1900	1908	rBV4	2492	4387	1.13%	0.145%
15	7.317	1941	1952	1972	rBV	191831	329259	85.15%	10.876%
16	7.397	1972	1977	1988	rVB6	2697	4649	1.20%	0.154%
17	7.625	2040	2048	2071	rBV2	24126	44015	11.38%	1.454%
18	8.098	2185	2195	2239	rBV2	118477	297429	76.92%	9.824%
19	8.854	2419	2430	2459	rBV	169563	281618	72.83%	9.302%
20	10.220	2844	2855	2870	rBV	54031	85029	21.99%	2.809%
21	11.249	3164	3175	3200	rBV	167310	266472	68.91%	8.802%
22	11.625	3280	3292	3311	rBV	181935	280135	72.44%	9.253%




Sum of corrected areas: 3027504

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023028.D
Acq On : 26 Oct 2021 10:39
Operator : SY/MD
Sample : VV1026WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

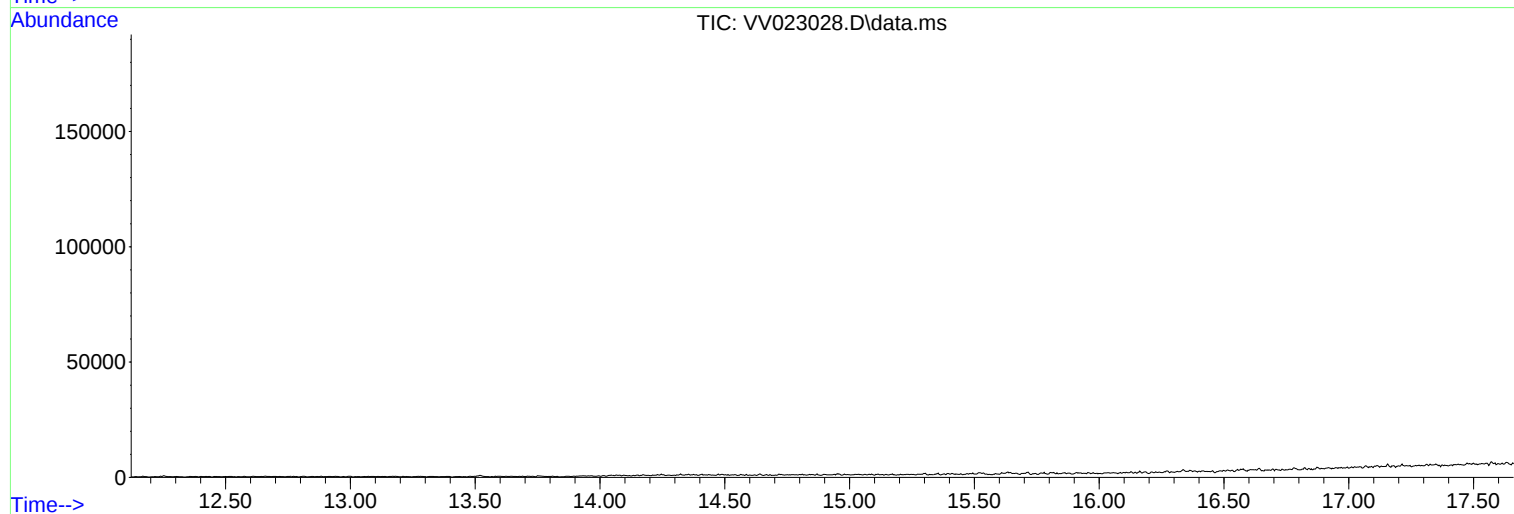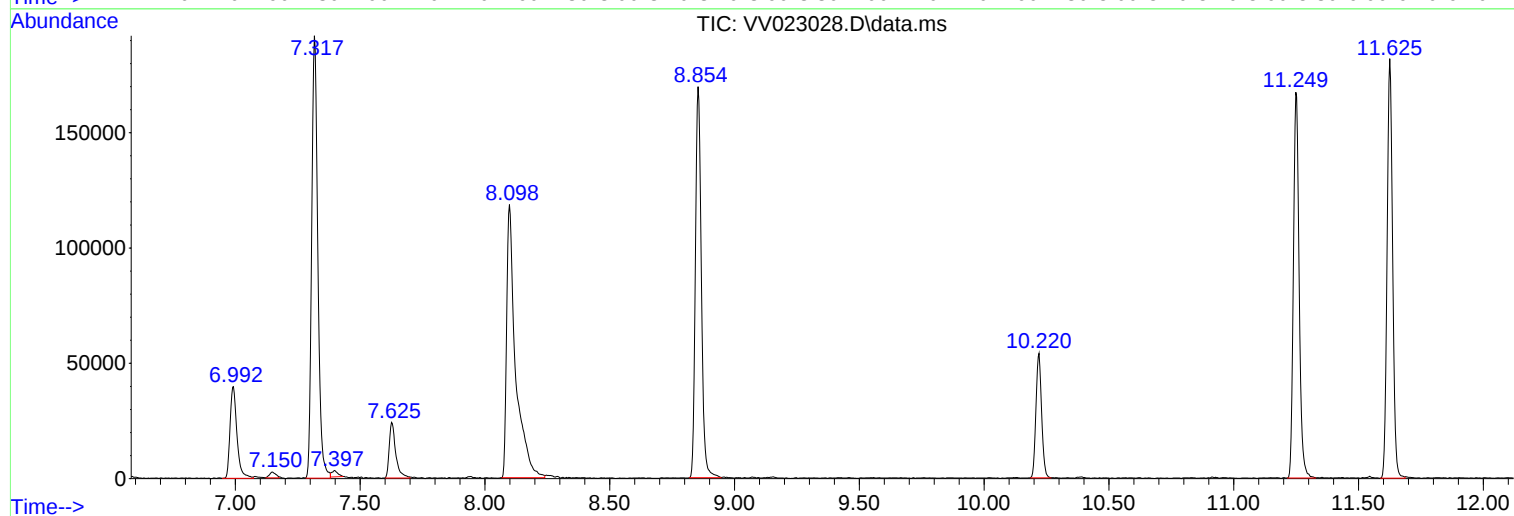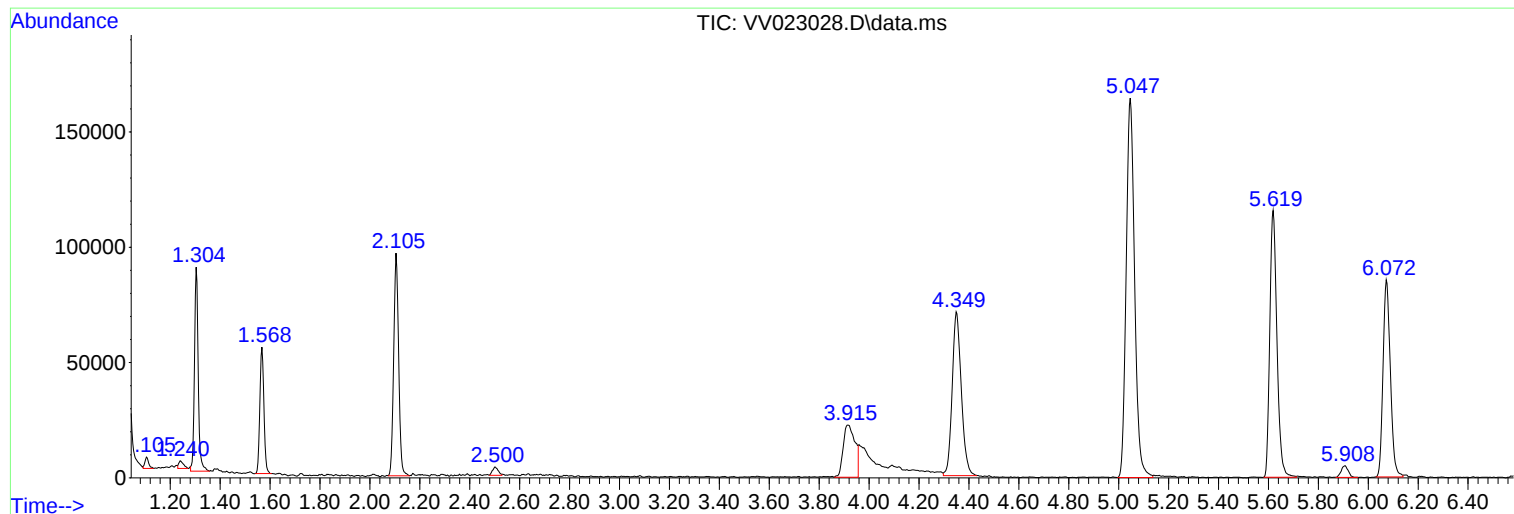

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023028.D
Acq On : 26 Oct 2021 10:39
Operator : SY/MD
Sample : VV1026WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023028.D
Acq On : 26 Oct 2021 10:39
Operator : SY/MD
Sample : VV1026WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc