

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023030.D
 Acq On : 26 Oct 2021 11:43
 Operator : SY/MD
 Sample : M4278-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023030.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rVB	80744	83954	16.65%	1.848%
2	1.568	156	164	175	rVB	65482	70207	13.92%	1.546%
3	2.108	322	332	346	rBV	92948	137893	27.34%	3.036%
4	2.178	346	354	368	rVB2	3711	7418	1.47%	0.163%
5	2.513	449	458	469	rVB7	2854	5468	1.08%	0.120%
6	2.767	527	537	539	rBV4	5752	6948	1.38%	0.153%
7	3.912	876	893	917	rBV3	106333	349398	69.29%	7.693%
8	4.355	1014	1031	1061	rBV2	85741	229494	45.51%	5.053%
9	5.053	1232	1248	1281	rBV2	200863	504283	100.00%	11.103%
10	5.622	1413	1425	1446	rBV2	147217	300402	59.57%	6.614%
11	5.921	1505	1518	1535	rBV5	37424	81494	16.16%	1.794%
12	6.072	1552	1565	1587	rBV	116027	239816	47.56%	5.280%
13	6.992	1840	1851	1873	rBV	52151	101679	20.16%	2.239%
14	7.320	1941	1953	1969	rBV	232723	403855	80.08%	8.892%
15	7.400	1971	1978	1987	rVB3	8263	14719	2.92%	0.324%
16	7.628	2038	2049	2065	rBV	31106	57553	11.41%	1.267%
17	7.979	2140	2158	2179	rBV	229315	379632	75.28%	8.359%
18	8.091	2183	2193	2231	rBV	195220	387738	76.89%	8.537%
19	8.853	2419	2430	2456	rBV	228425	384406	76.23%	8.464%
20	9.146	2514	2521	2532	rVB5	3238	5387	1.07%	0.119%
21	10.217	2842	2854	2872	rBV	73735	119736	23.74%	2.636%
22	11.249	3165	3175	3191	rBV	207287	329761	65.39%	7.261%
23	11.625	3278	3292	3311	rBV	212948	340536	67.53%	7.498%




Sum of corrected areas: 4541777

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023030.D
Acq On : 26 Oct 2021 11:43
Operator : SY/MD
Sample : M4278-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

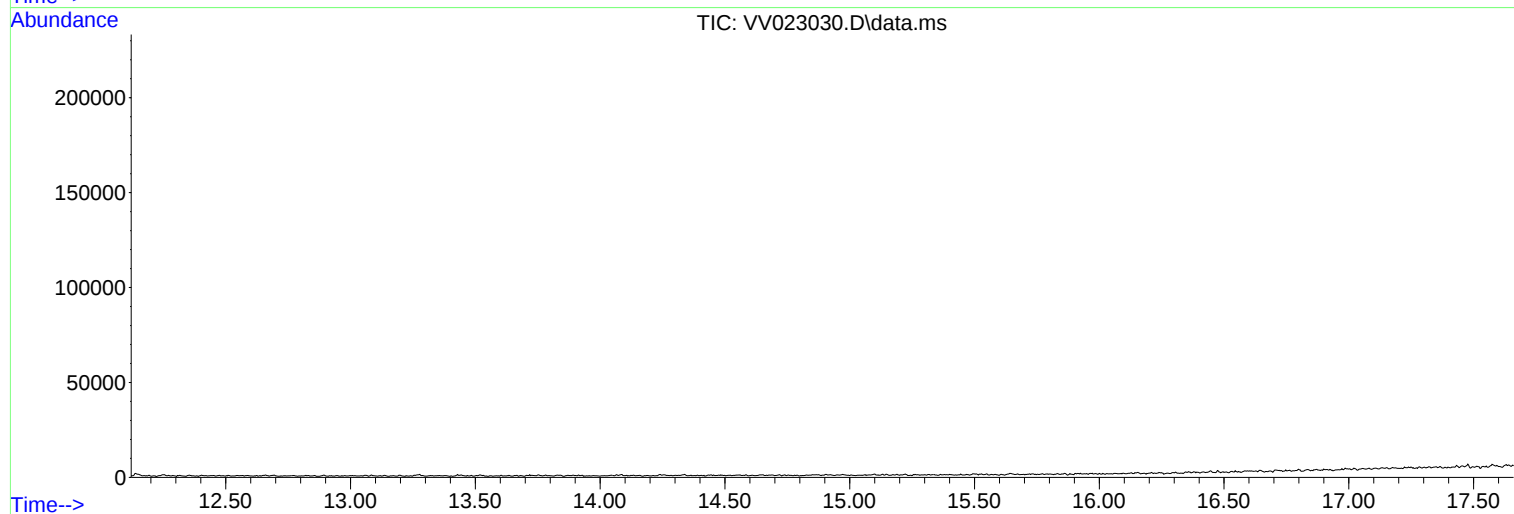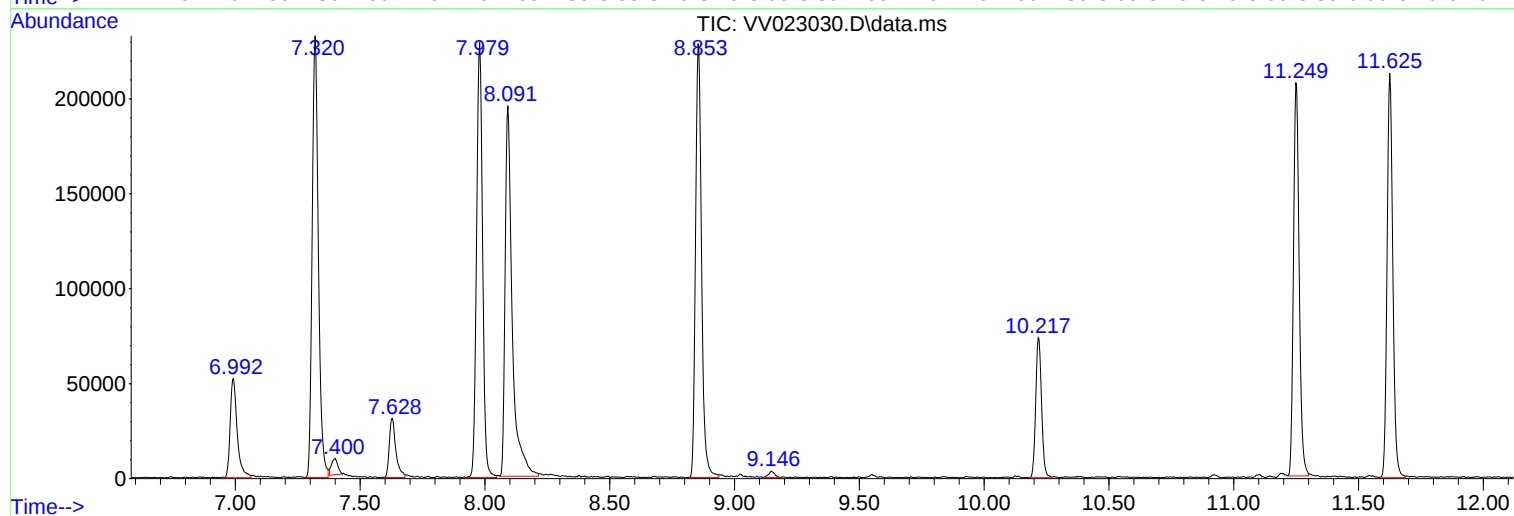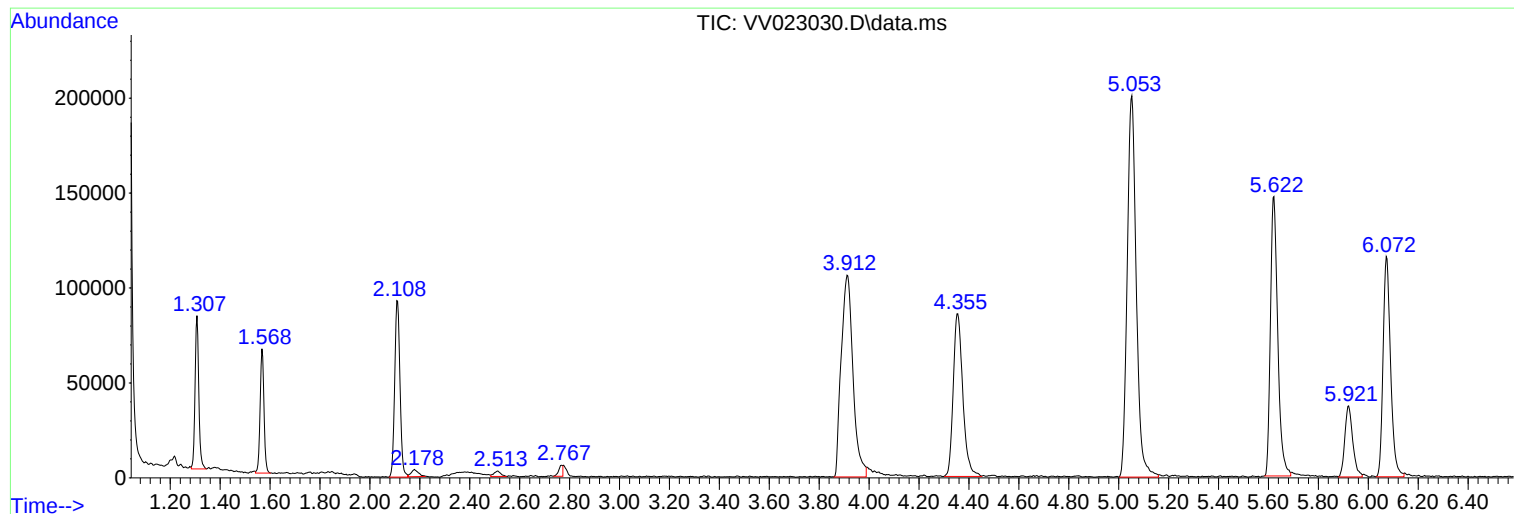

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023030.D
Acq On : 26 Oct 2021 11:43
Operator : SY/MD
Sample : M4278-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023030.D
Acq On : 26 Oct 2021 11:43
Operator : SY/MD
Sample : M4278-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc