

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023032.D
 Acq On : 26 Oct 2021 12:29
 Operator : SY/MD
 Sample : M4265-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023032.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	97	rVB	87078	90818	16.65%	2.222%
2	1.568	156	164	172	rBV	60436	67117	12.31%	1.642%
3	2.108	322	332	350	rBV	107499	156278	28.66%	3.824%
4	2.510	449	457	468	rVB6	4245	7666	1.41%	0.188%
5	3.889	876	886	918	rBV2	56361	171523	31.45%	4.198%
6	4.352	1010	1030	1059	rBV	94201	244157	44.77%	5.975%
7	5.050	1231	1247	1278	rBV2	214547	545310	100.00%	13.345%
8	5.619	1410	1424	1445	rBV	148066	300160	55.04%	7.346%
9	5.918	1506	1517	1530	rVB10	4060	9857	1.81%	0.241%
10	6.072	1553	1565	1587	rBV	124245	257914	47.30%	6.312%
11	6.989	1839	1850	1873	rBV2	56094	108259	19.85%	2.649%
12	7.317	1937	1952	1971	rBV	250966	440326	80.75%	10.776%
13	7.394	1973	1976	1988	rVB6	3873	6588	1.21%	0.161%
14	7.625	2038	2048	2072	rBV	33861	63061	11.56%	1.543%
15	8.092	2180	2193	2225	rBV2	213928	424446	77.84%	10.387%
16	8.854	2417	2430	2450	rBV	224230	374335	68.65%	9.161%
17	10.217	2842	2854	2871	rBV	79703	128588	23.58%	3.147%
18	10.384	2897	2906	2916	rVB2	3832	5740	1.05%	0.140%
19	11.249	3164	3175	3196	rBV	207087	323790	59.38%	7.924%
20	11.625	3281	3292	3312	rBV	225683	360374	66.09%	8.819%




Sum of corrected areas: 4086307

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023032.D
Acq On : 26 Oct 2021 12:29
Operator : SY/MD
Sample : M4265-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

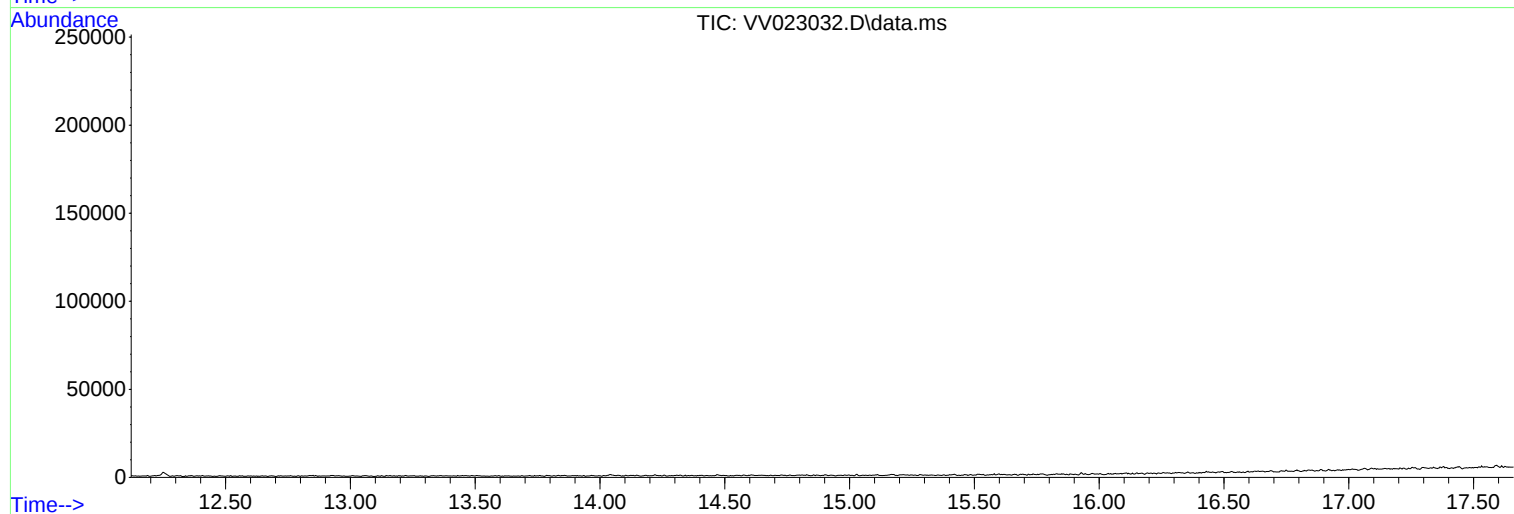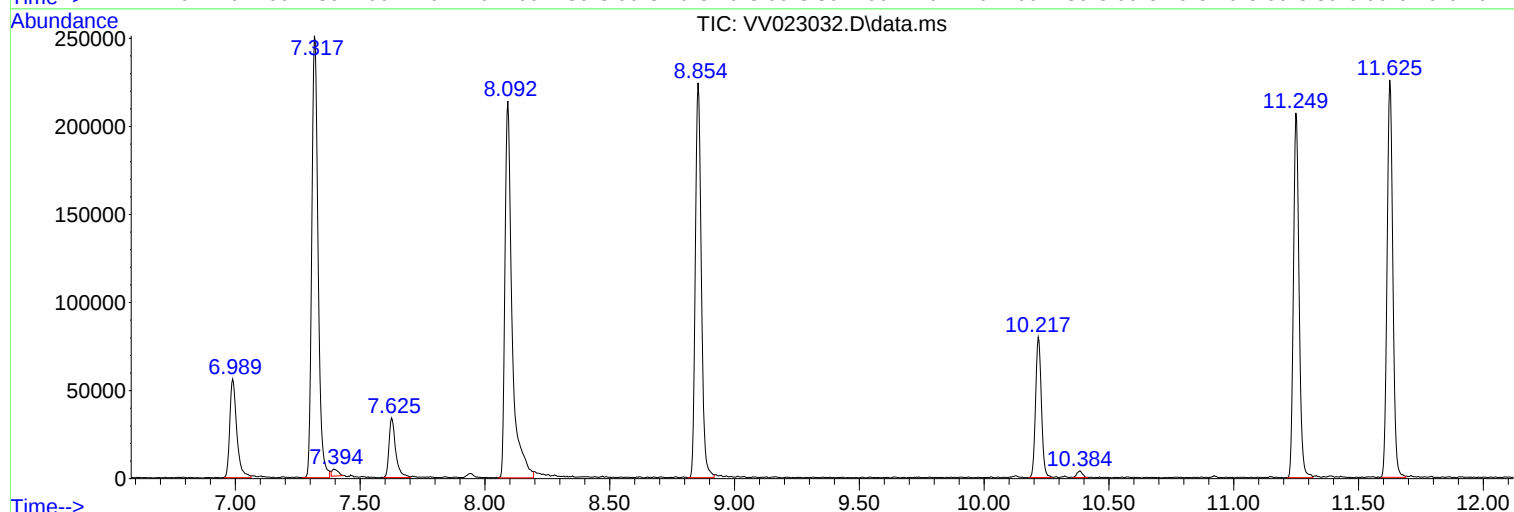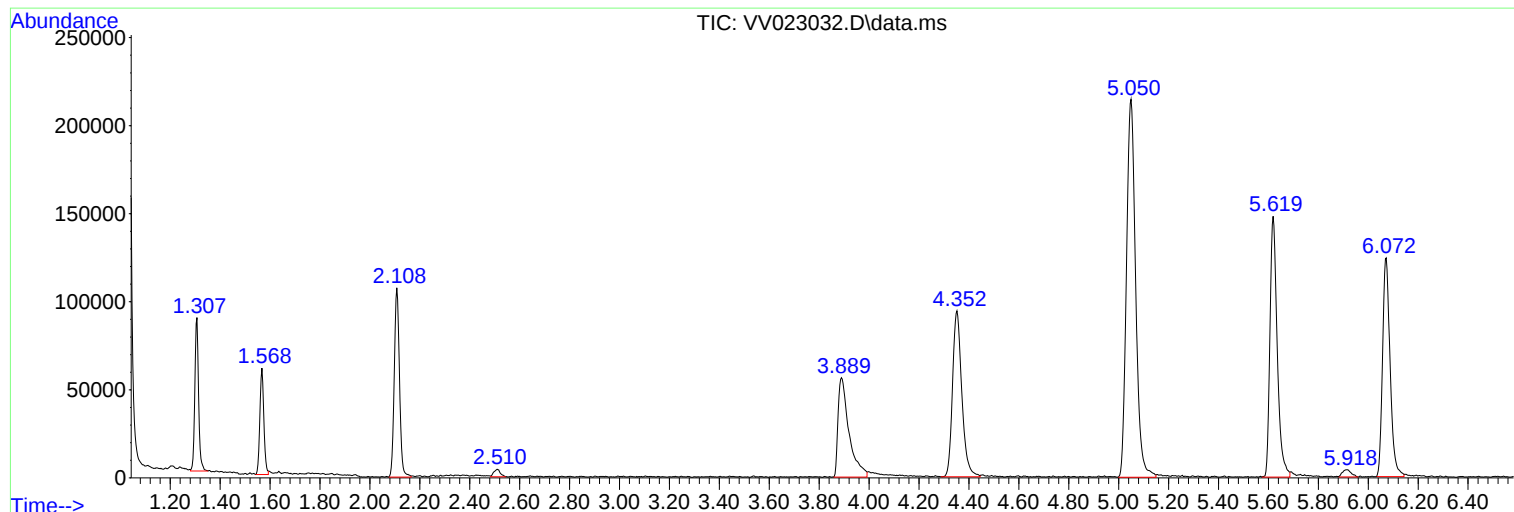

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023032.D
Acq On : 26 Oct 2021 12:29
Operator : SY/MD
Sample : M4265-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023032.D
Acq On : 26 Oct 2021 12:29
Operator : SY/MD
Sample : M4265-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc