

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023036.D
 Acq On : 26 Oct 2021 14:04
 Operator : SY/MD
 Sample : M4278-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGH0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023036.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.217	52	55	63	rVB2	5320	4930	1.12%	0.109%
2	1.307	75	83	94	rVB	85483	90811	20.60%	2.016%
3	1.568	156	164	177	rBV	58999	66484	15.08%	1.476%
4	2.108	320	332	345	rBV	97319	139505	31.65%	3.097%
5	2.185	345	356	372	rVB	4378	11435	2.59%	0.254%
6	2.770	527	538	551	rVB2	4041	8191	1.86%	0.182%
7	3.908	877	892	927	rBV5	84728	278948	63.29%	6.192%
8	4.352	1010	1030	1056	rBV	73190	190151	43.14%	4.221%
9	5.050	1228	1247	1278	rBV2	177311	440777	100.00%	9.785%
10	5.619	1411	1424	1449	rBV	132497	270223	61.31%	5.999%
11	5.918	1503	1517	1537	rBV4	34106	73477	16.67%	1.631%
12	6.072	1552	1565	1591	rBV	101096	208408	47.28%	4.626%
13	6.989	1840	1850	1878	rBV2	49422	93294	21.17%	2.071%
14	7.317	1940	1952	1970	rBV	239287	425041	96.43%	9.435%
15	7.394	1971	1976	1994	rVB2	8507	17107	3.88%	0.380%
16	7.625	2038	2048	2070	rBV2	33839	63189	14.34%	1.403%
17	7.976	2145	2157	2179	rBV	261428	438779	99.55%	9.740%
18	8.092	2182	2193	2223	rBV2	215053	429362	97.41%	9.531%
19	8.854	2419	2430	2452	rBV	245509	406708	92.27%	9.028%
20	9.146	2514	2521	2533	rBV6	3001	4855	1.10%	0.108%
21	10.217	2843	2854	2875	rBV	78747	127541	28.94%	2.831%
22	11.249	3164	3175	3195	rVV	222937	347321	78.80%	7.710%
23	11.625	3281	3292	3311	rBV	229074	368223	83.54%	8.174%




Sum of corrected areas: 4504760

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023036.D
Acq On : 26 Oct 2021 14:04
Operator : SY/MD
Sample : M4278-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

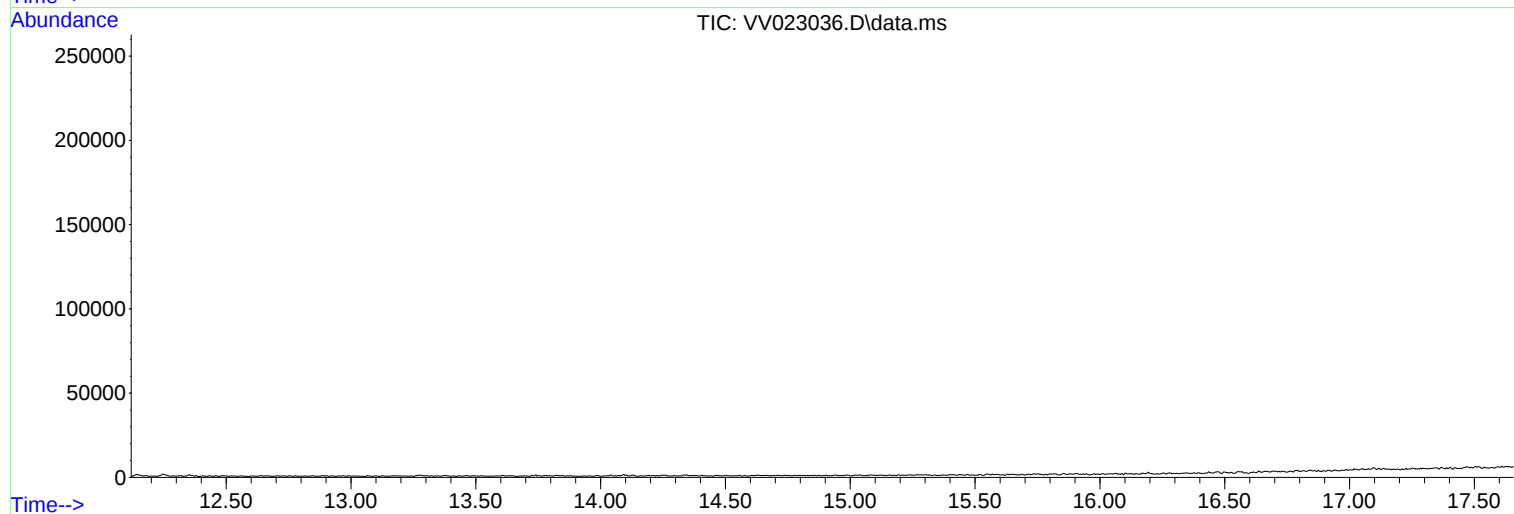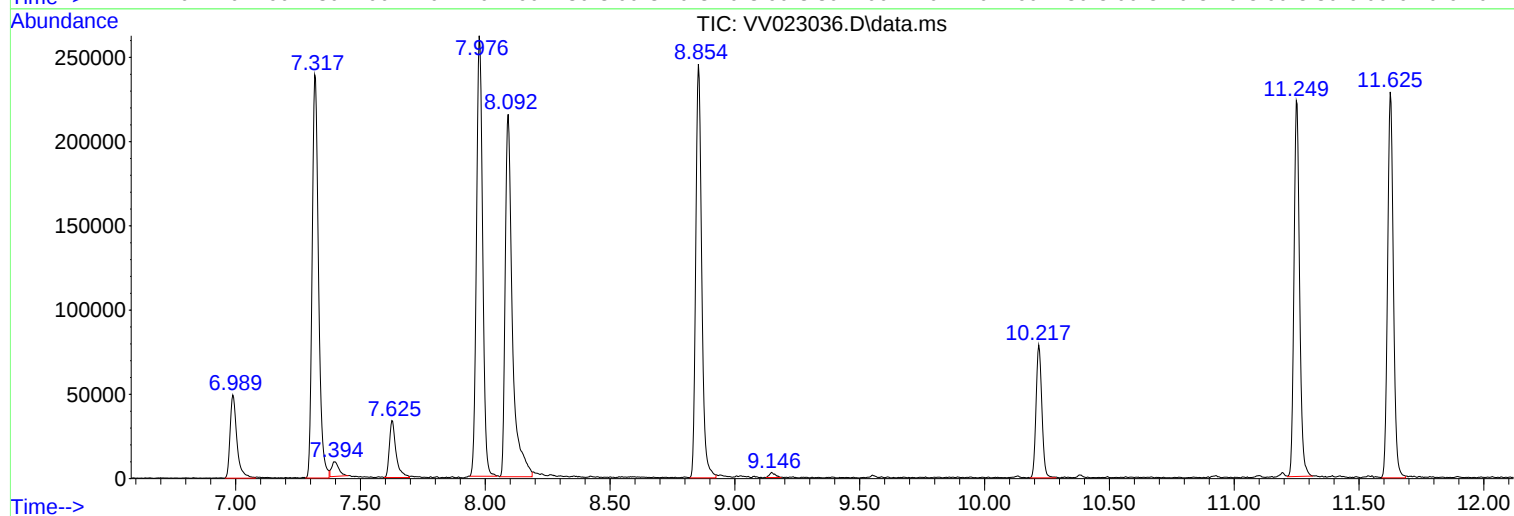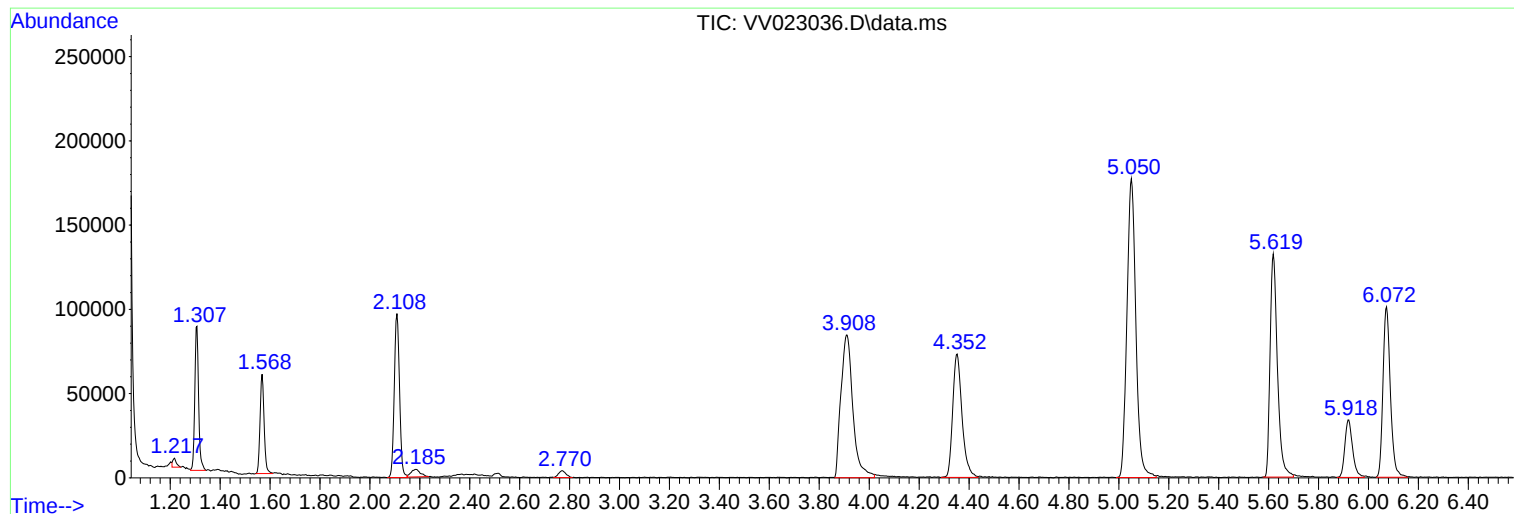

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023036.D
Acq On : 26 Oct 2021 14:04
Operator : SY/MD
Sample : M4278-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023036.D
Acq On : 26 Oct 2021 14:04
Operator : SY/MD
Sample : M4278-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc