

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023043.D
 Acq On : 26 Oct 2021 17:15
 Operator : SY/MD
 Sample : M4277-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGEO

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023043.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	75	83	100	rVB	92879	104301	23.84%	2.548%
2	1.568	156	164	176	rVB	49348	54877	12.54%	1.341%
3	2.108	321	332	344	rBV	97669	135607	30.99%	3.313%
4	2.178	344	354	382	rVB	16091	41974	9.59%	1.025%
5	3.912	876	893	915	rBV4	98551	301415	68.88%	7.363%
6	4.352	1014	1030	1057	rBV	62947	172549	39.43%	4.215%
7	5.050	1231	1247	1272	rBV2	157952	398086	90.97%	9.724%
8	5.619	1413	1424	1455	rBV	137563	284633	65.05%	6.953%
9	5.924	1507	1519	1528	rBV9	7171	14973	3.42%	0.366%
10	6.072	1550	1565	1582	rBV	122663	254020	58.05%	6.205%
11	6.989	1838	1850	1874	rBV	56268	108123	24.71%	2.641%
12	7.317	1939	1952	1971	rBV	248154	437590	100.00%	10.689%
13	7.397	1971	1977	1989	rVB3	8599	15787	3.61%	0.386%
14	7.625	2038	2048	2067	rBV	32957	61923	14.15%	1.513%
15	7.979	2150	2158	2171	rVB4	10275	17165	3.92%	0.419%
16	8.091	2183	2193	2231	rBV2	213360	431313	98.57%	10.536%
17	8.853	2417	2430	2449	rBV	233444	388320	88.74%	9.486%
18	9.143	2512	2520	2533	rBV5	5168	8258	1.89%	0.202%
19	9.866	2736	2745	2756	rBV6	6254	11378	2.60%	0.278%
20	10.217	2844	2854	2874	rBV	82992	132573	30.30%	3.239%
21	10.722	3004	3011	3024	rBV5	2855	5542	1.27%	0.135%
22	11.098	3120	3128	3137	rVB3	3585	5677	1.30%	0.139%
23	11.249	3165	3175	3197	rVB	215326	339442	77.57%	8.292%
24	11.625	3279	3292	3310	rBV	227164	368120	84.12%	8.992%




Sum of corrected areas: 4093646

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023043.D
Acq On : 26 Oct 2021 17:15
Operator : SY/MD
Sample : M4277-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

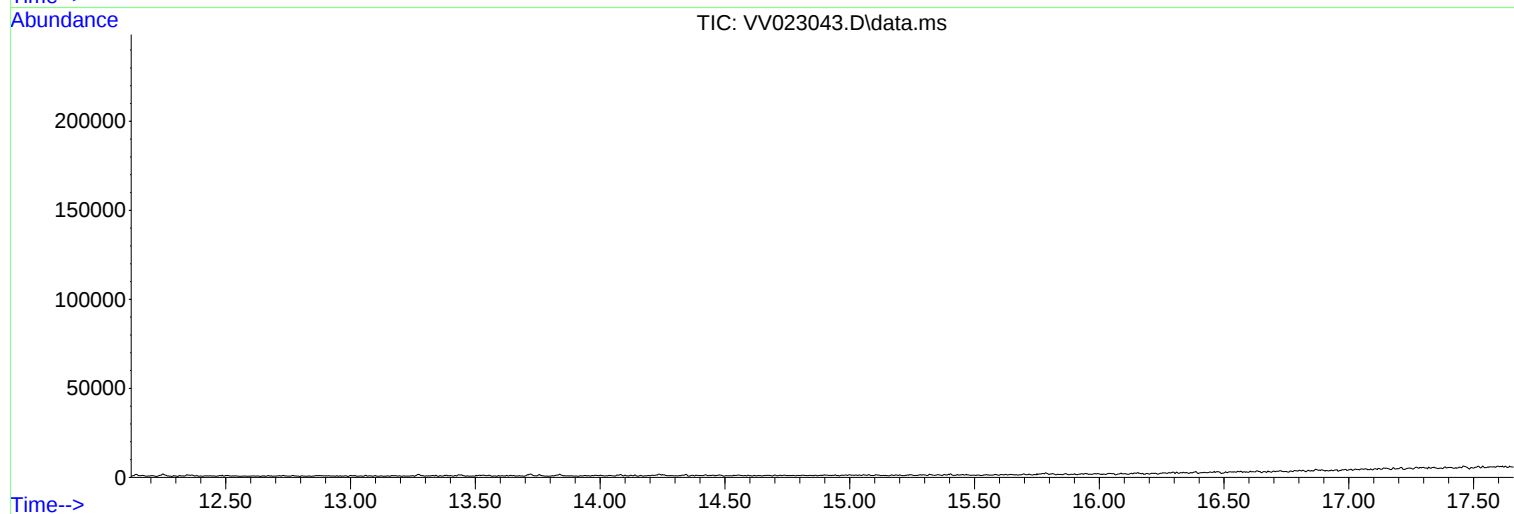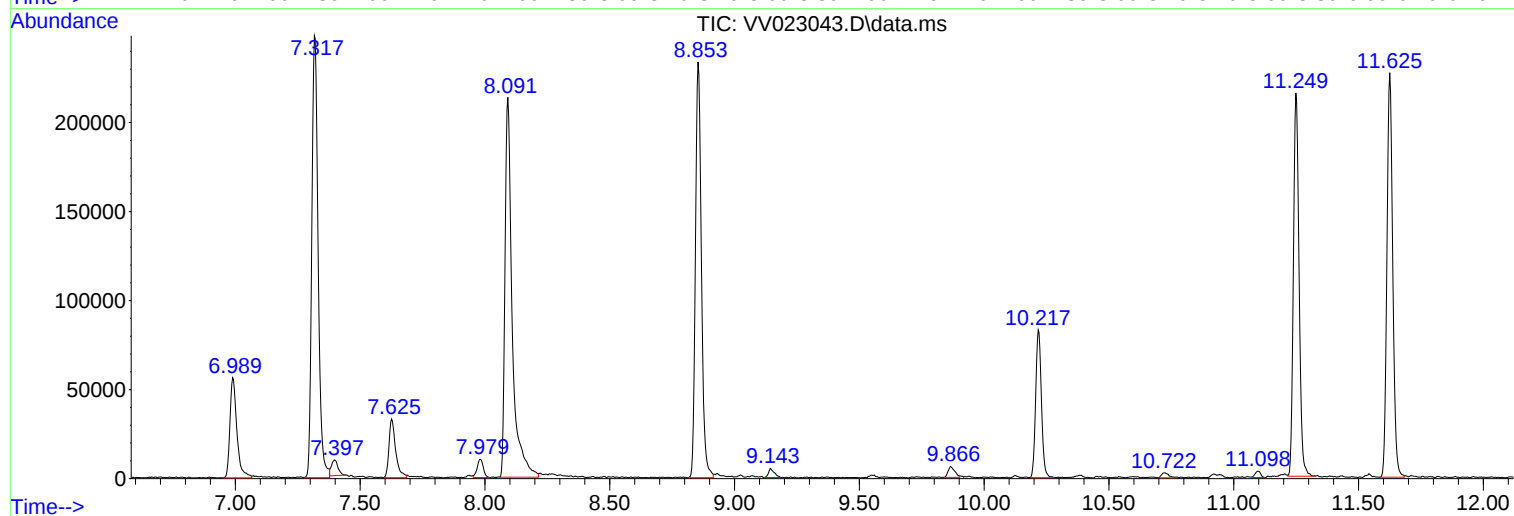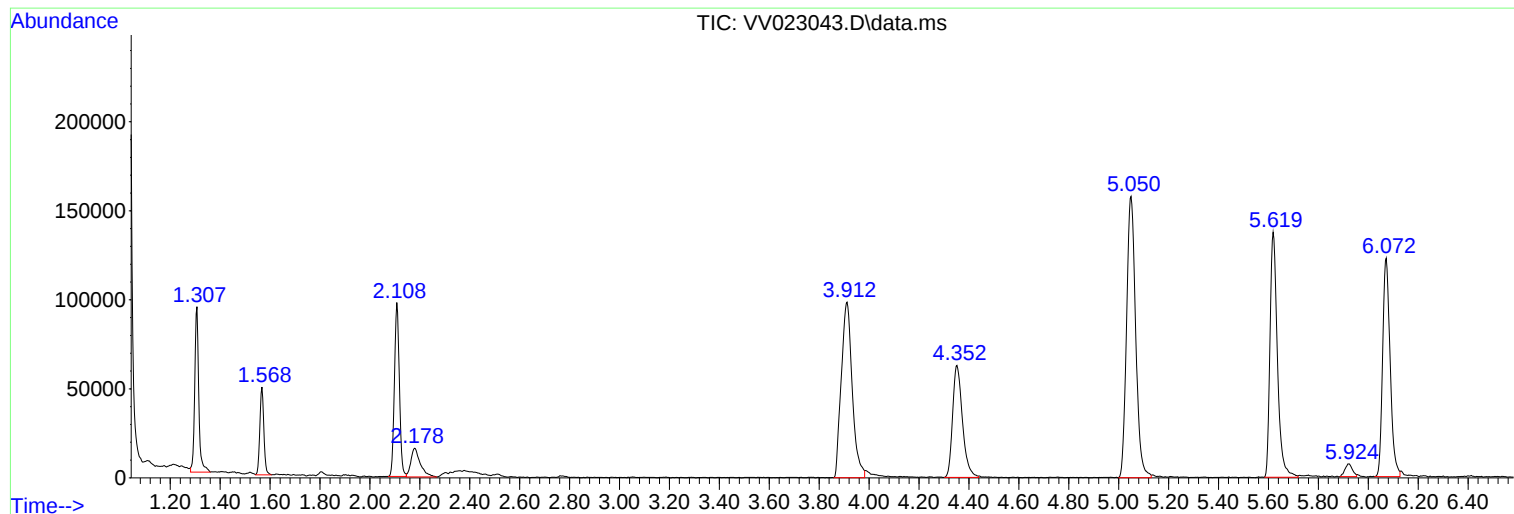

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023043.D
Acq On : 26 Oct 2021 17:15
Operator : SY/MD
Sample : M4277-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023043.D
Acq On : 26 Oct 2021 17:15
Operator : SY/MD
Sample : M4277-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc