

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023044.D
 Acq On : 26 Oct 2021 17:39
 Operator : SY/MD
 Sample : M4277-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGES

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023044.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.105	15	20	31	rVB2	17924	18828	3.53%	0.385%
2	1.201	45	50	59	rBV3	5555	6307	1.18%	0.129%
3	1.307	75	83	97	rVB	87374	96282	18.03%	1.970%
4	1.568	156	164	176	rVB	58141	68081	12.75%	1.393%
5	1.632	176	184	191	rBV5	3665	5377	1.01%	0.110%
6	2.108	320	332	344	rBV	105648	152939	28.64%	3.130%
7	2.172	347	352	367	rVB3	3377	6889	1.29%	0.141%
8	2.349	382	407	408	rBV	14705	41761	7.82%	0.855%
9	2.767	523	537	561	rBV	88134	189214	35.43%	3.872%
10	3.741	826	840	842	rBV4	6546	11122	2.08%	0.228%
11	3.886	874	885	912	rBV	59424	187094	35.03%	3.829%
12	4.352	1013	1030	1064	rBV	92461	254614	47.68%	5.211%
13	5.050	1231	1247	1275	rBV2	210604	534025	100.00%	10.929%
14	5.619	1412	1424	1456	rBV	153340	320255	59.97%	6.554%
15	5.921	1505	1518	1539	rVB7	8329	21641	4.05%	0.443%
16	6.072	1552	1565	1587	rBV2	123953	257010	48.13%	5.260%
17	6.989	1839	1850	1868	rBV	55828	105678	19.79%	2.163%
18	7.317	1939	1952	1970	rBV	246054	433196	81.12%	8.865%
19	7.397	1970	1977	1989	rVB2	8340	16028	3.00%	0.328%
20	7.625	2038	2048	2073	rBV	32843	62259	11.66%	1.274%
21	7.976	2144	2157	2180	rVB	254182	434406	81.35%	8.890%
22	8.092	2183	2193	2223	rBV	227073	436043	81.65%	8.924%
23	8.854	2418	2430	2451	rBV	238109	393026	73.60%	8.043%
24	10.217	2843	2854	2871	rBV	83439	134240	25.14%	2.747%
25	11.249	3164	3175	3194	rBV	217457	339663	63.60%	6.951%
26	11.625	3280	3292	3310	rBV	226041	360430	67.49%	7.376%




Sum of corrected areas: 4886408

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023044.D
Acq On : 26 Oct 2021 17:39
Operator : SY/MD
Sample : M4277-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

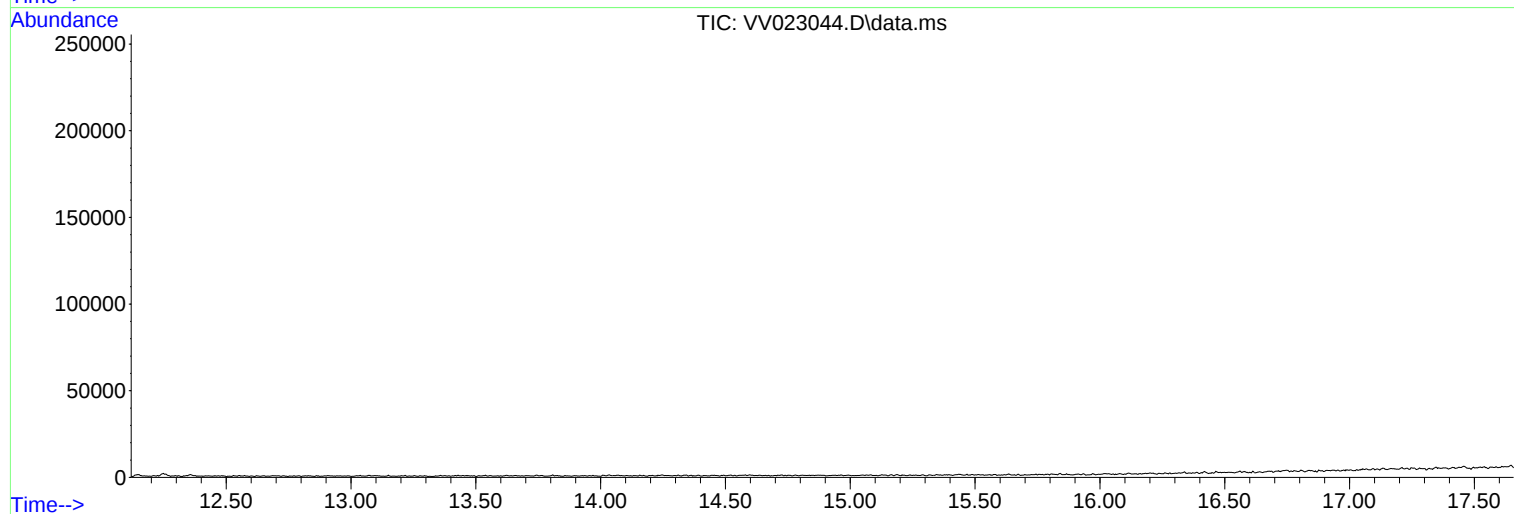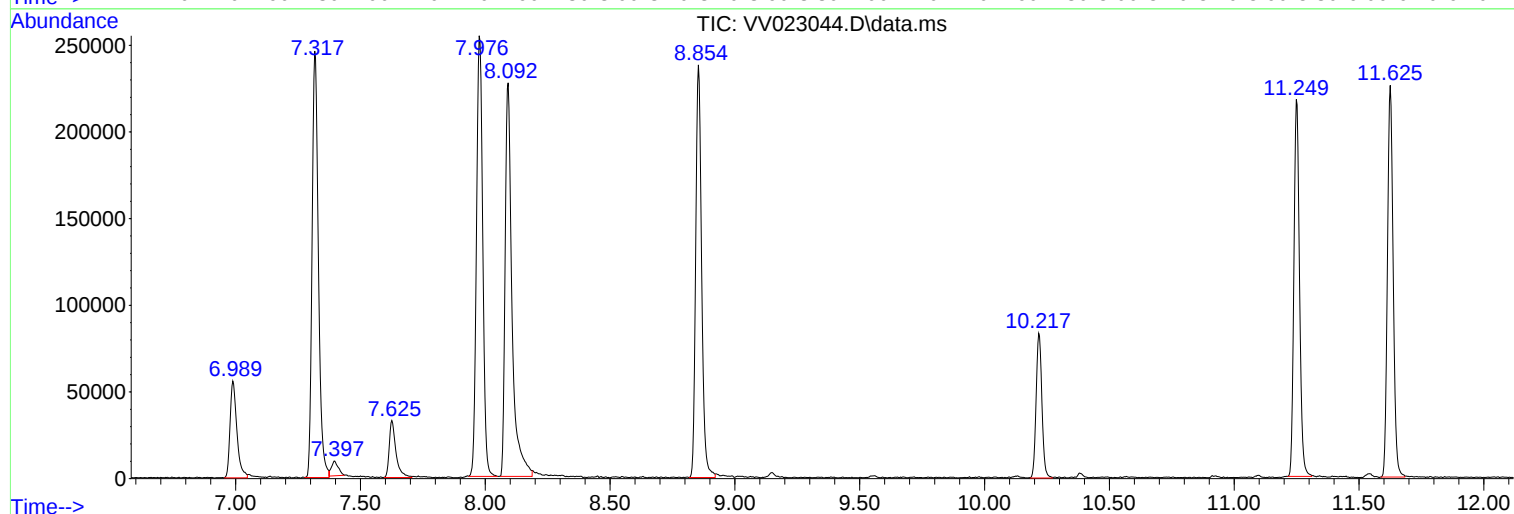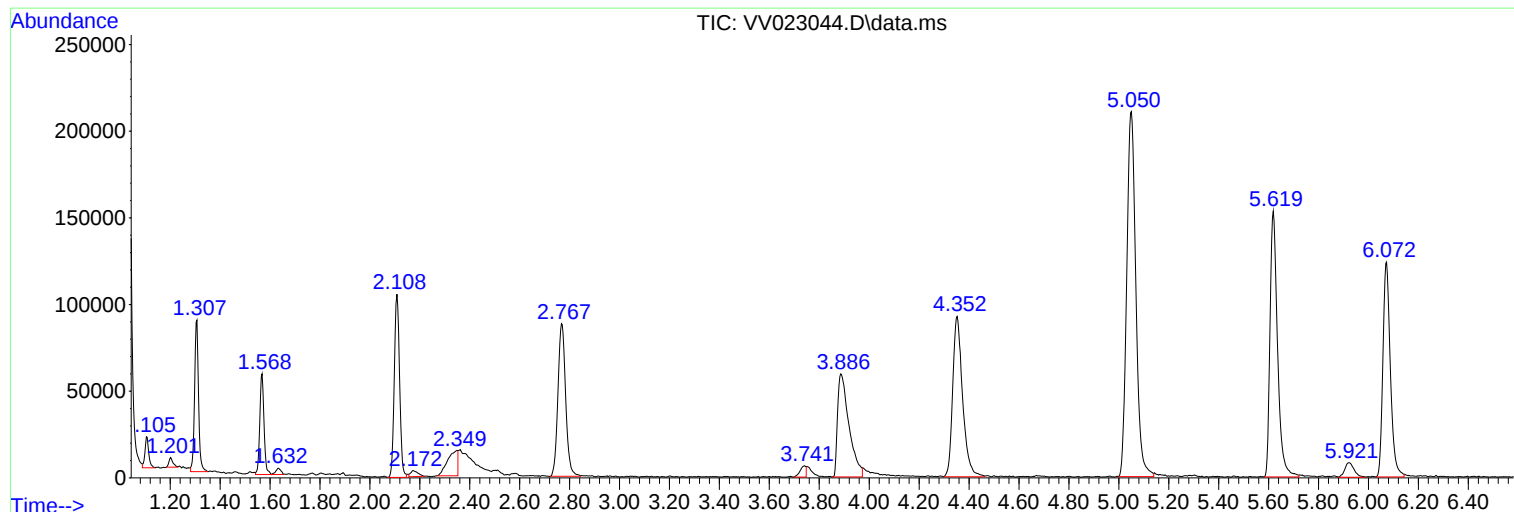

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023044.D
Acq On : 26 Oct 2021 17:39
Operator : SY/MD
Sample : M4277-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFG5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.349	0.65 ug/L	41761	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	43
2			2-Propanone, 1-methoxy-	88	C4H8O2	005878-19-3	9
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	9
5			Oxirane, (methoxymethyl)-	88	C4H8O2	000930-37-0	4

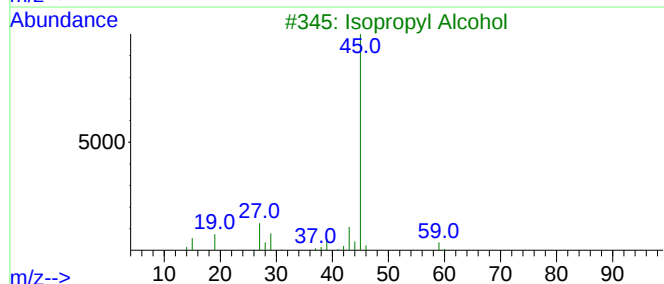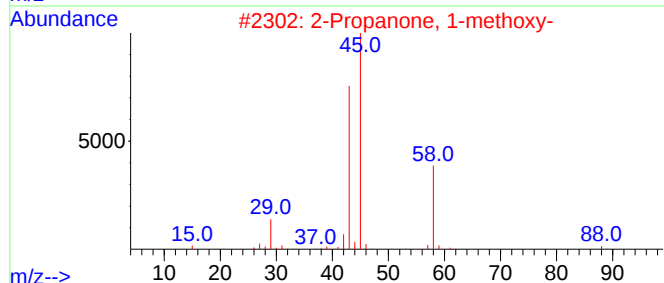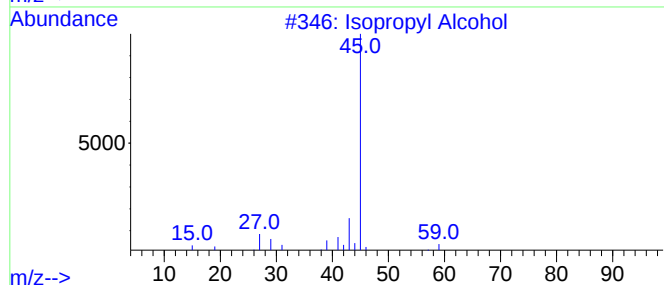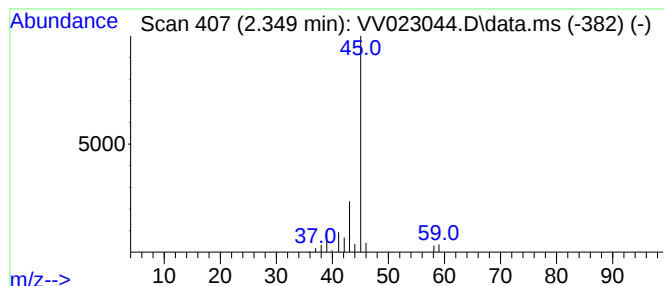

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023044.D
Acq On : 26 Oct 2021 17:39
Operator : SY/MD
Sample : M4277-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	2.349	0.7	ug/L	41761	1	5.619	320255	5.0