

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023045.D
 Acq On : 26 Oct 2021 18:03
 Operator : SY/MD
 Sample : M4277-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGA7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023045.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	99	rVB	90277	96504	9.07%	1.599%
2	1.568	156	164	174	rVB	52223	58636	5.51%	0.972%
3	2.108	318	332	347	rBV	97814	143459	13.49%	2.377%
4	2.770	524	538	553	rBV3	8979	18406	1.73%	0.305%
5	3.912	876	893	920	rBV3	287883	806006	75.77%	13.354%
6	4.352	1011	1030	1060	rBV	90405	247824	23.30%	4.106%
7	5.050	1231	1247	1276	rBV2	214628	540306	50.80%	8.952%
8	5.619	1410	1424	1452	rBV	153555	321601	30.23%	5.328%
9	5.918	1505	1517	1540	rBV	82159	166063	15.61%	2.751%
10	6.072	1552	1565	1590	rBV	120808	255972	24.06%	4.241%
11	6.989	1840	1850	1870	rBV	56590	107538	10.11%	1.782%
12	7.317	1939	1952	1970	rBV	245195	431256	40.54%	7.145%
13	7.397	1971	1977	1989	rVB	7688	15152	1.42%	0.251%
14	7.625	2037	2048	2071	rBV2	34270	63570	5.98%	1.053%
15	7.976	2137	2157	2180	rBV	629848	1063688	100.00%	17.624%
16	8.091	2183	2193	2229	rVV	227540	442197	41.57%	7.327%
17	8.853	2419	2430	2452	rBV	243086	397913	37.41%	6.593%
18	10.217	2843	2854	2868	rBV	84796	133426	12.54%	2.211%
19	11.249	3164	3175	3197	rVB	227090	356168	33.48%	5.901%
20	11.625	3281	3292	3312	rBV	226277	369804	34.77%	6.127%




Sum of corrected areas: 6035489

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023045.D
Acq On : 26 Oct 2021 18:03
Operator : SY/MD
Sample : M4277-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

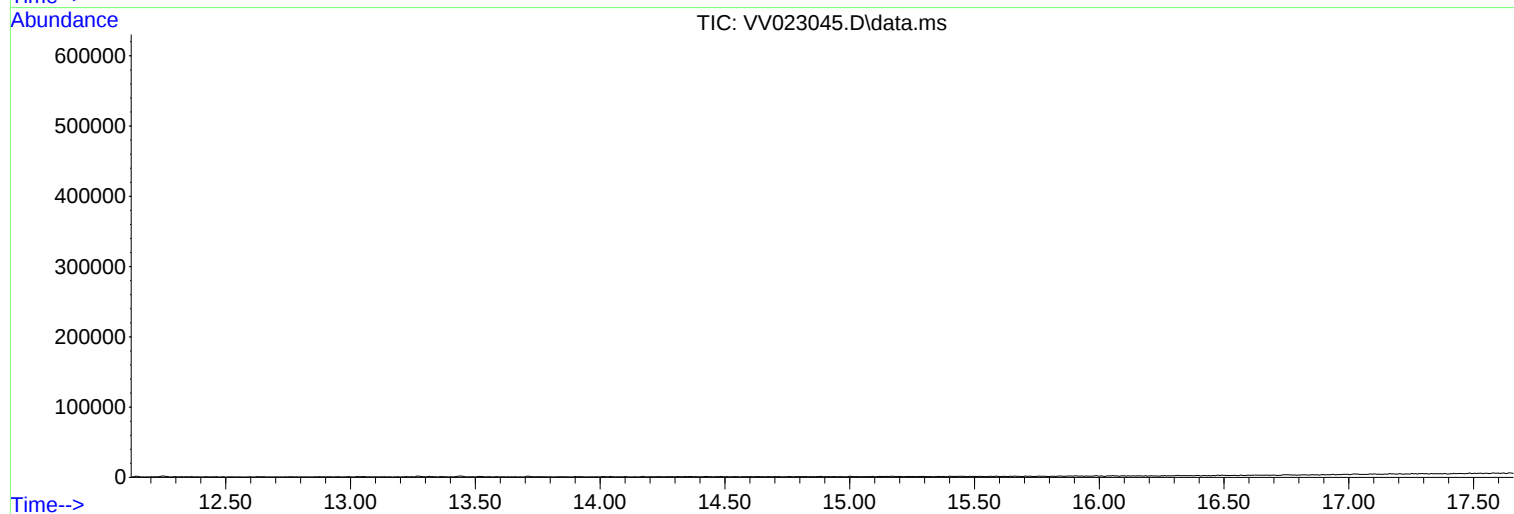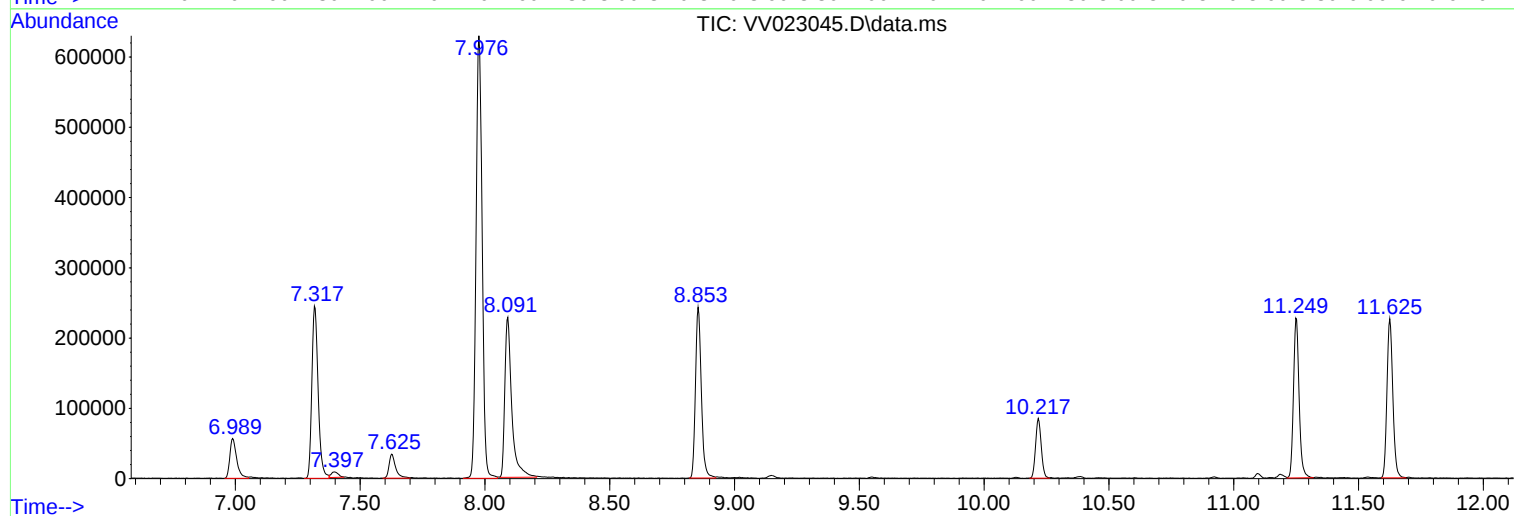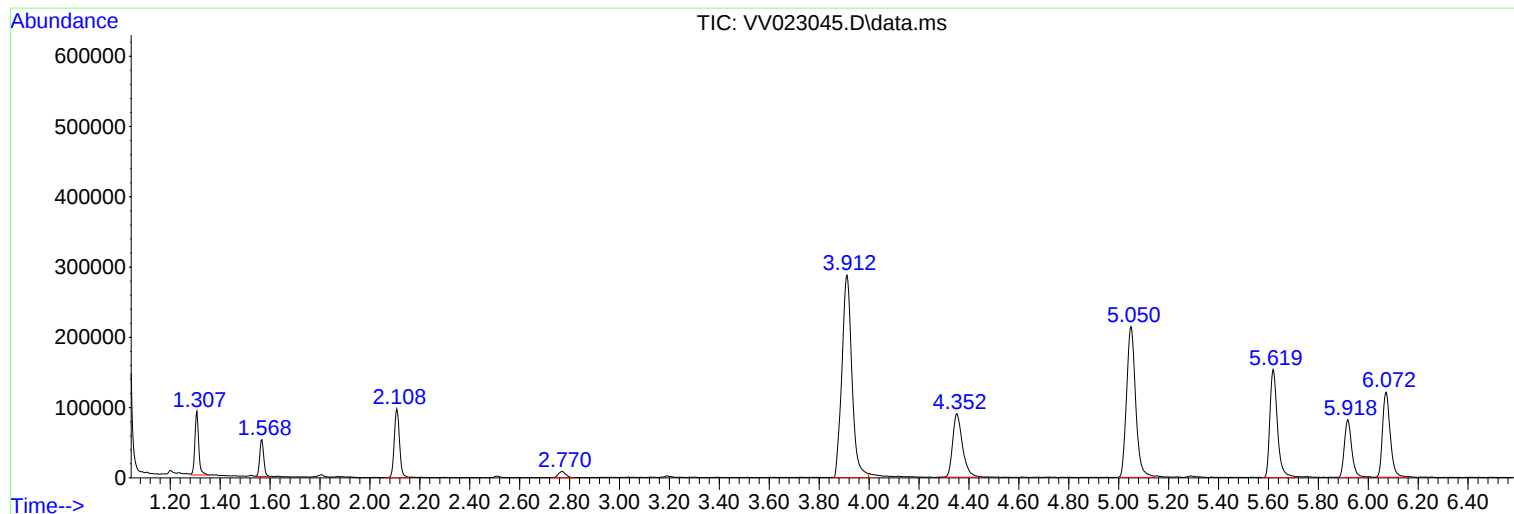

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023045.D
Acq On : 26 Oct 2021 18:03
Operator : SY/MD
Sample : M4277-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023045.D
Acq On : 26 Oct 2021 18:03
Operator : SY/MD
Sample : M4277-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
