

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023047.D
 Acq On : 26 Oct 2021 18:50
 Operator : SY/MD
 Sample : M4277-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023047.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	92	rVB	78776	79348	18.94%	2.016%
2	1.568	156	164	180	rVB	48132	54587	13.03%	1.387%
3	2.108	319	332	343	rBV	95177	139232	33.23%	3.538%
4	2.179	343	354	385	rVB2	30886	85766	20.47%	2.179%
5	3.908	877	892	914	rBV4	58777	200507	47.85%	5.095%
6	4.352	1013	1030	1065	rBV2	71417	190182	45.39%	4.833%
7	5.050	1230	1247	1274	rBV2	169252	419036	100.00%	10.648%
8	5.619	1411	1424	1445	rBV	131610	269968	64.43%	6.860%
9	5.921	1504	1518	1532	rBV7	8729	19954	4.76%	0.507%
10	6.072	1551	1565	1590	rBV2	97671	203863	48.65%	5.180%
11	6.989	1837	1850	1870	rBV	52325	100737	24.04%	2.560%
12	7.320	1939	1953	1969	rBV	229064	405518	96.77%	10.305%
13	7.400	1972	1978	1991	rVB	6457	12439	2.97%	0.316%
14	7.625	2038	2048	2065	rBV	30596	57555	13.74%	1.463%
15	7.979	2147	2158	2178	rVB	56048	96389	23.00%	2.449%
16	8.091	2183	2193	2227	rBV	203005	405357	96.74%	10.301%
17	8.854	2418	2430	2456	rBV	238742	397271	94.81%	10.095%
18	10.217	2843	2854	2866	rBV	76815	122967	29.35%	3.125%
19	11.249	3165	3175	3194	rBV	218759	338444	80.77%	8.600%
20	11.625	3279	3292	3313	rBV	210681	336111	80.21%	8.541%




Sum of corrected areas: 3935231

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023047.D
Acq On : 26 Oct 2021 18:50
Operator : SY/MD
Sample : M4277-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

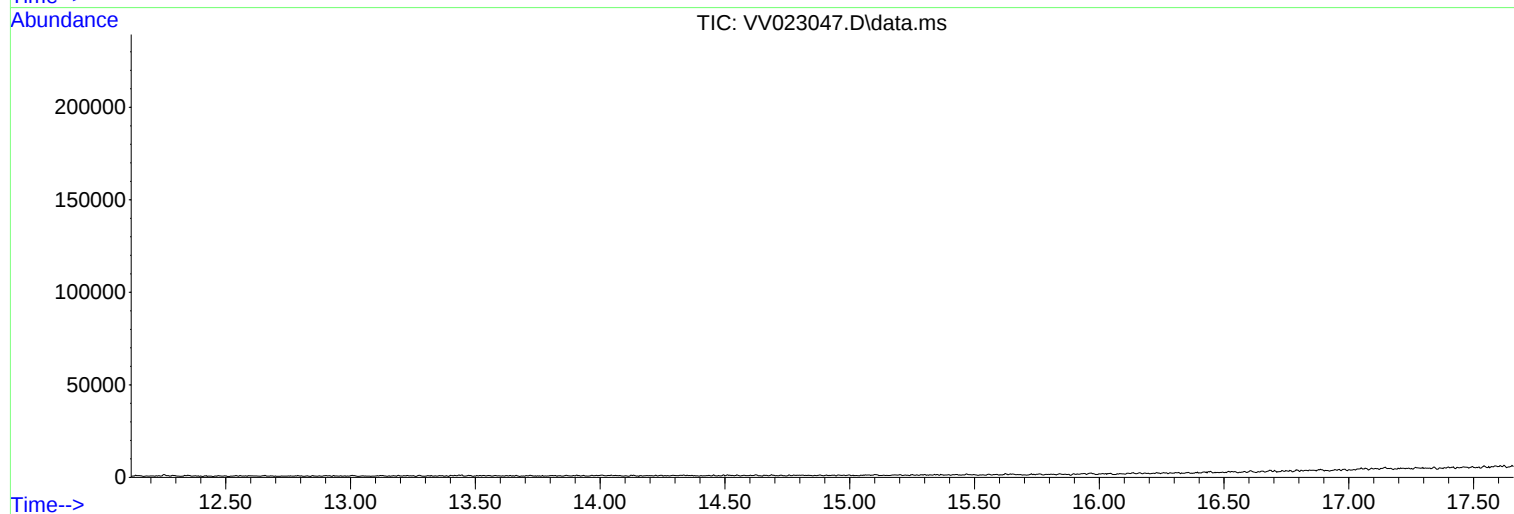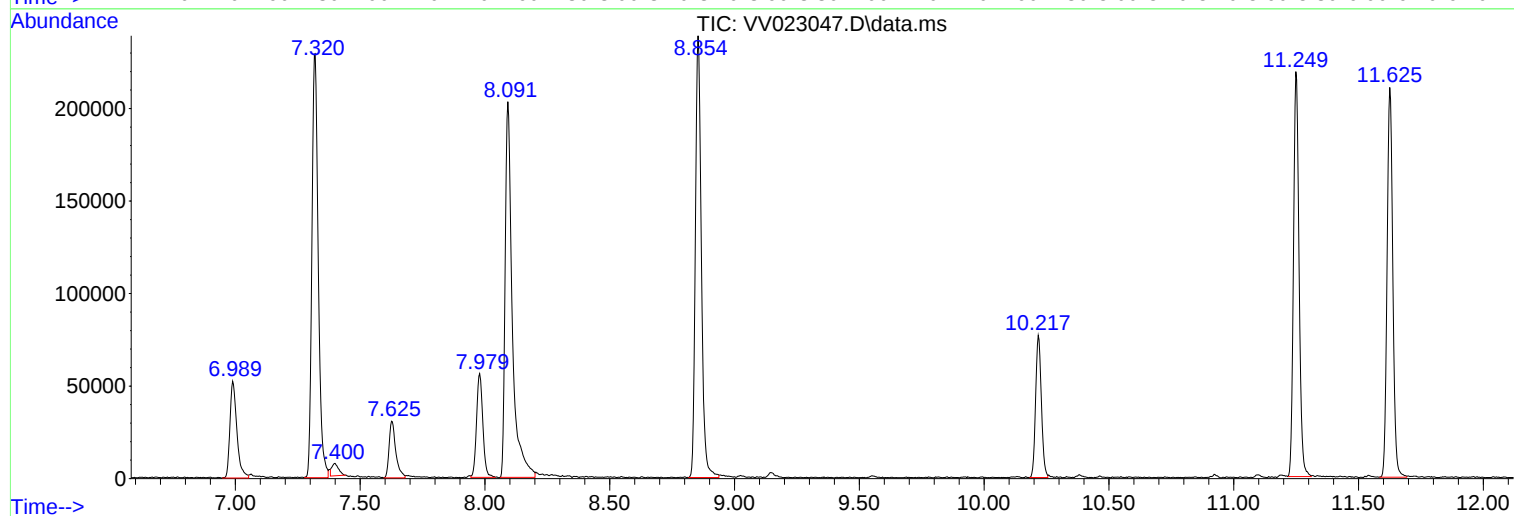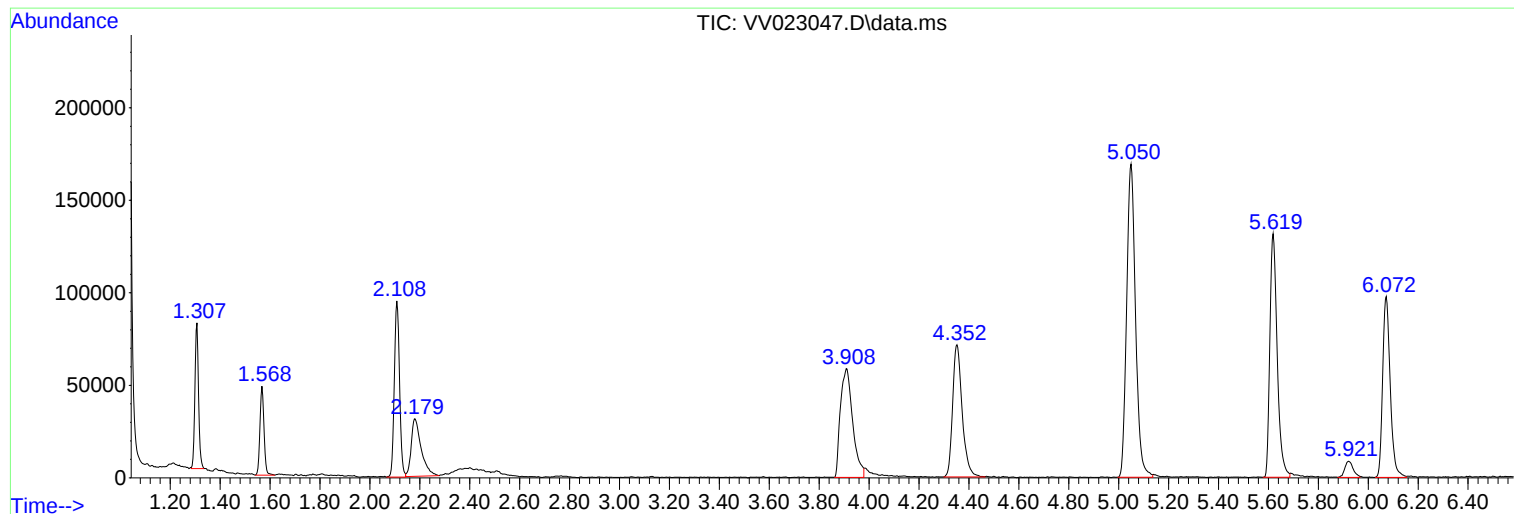

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023047.D
Acq On : 26 Oct 2021 18:50
Operator : SY/MD
Sample : M4277-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023047.D
Acq On : 26 Oct 2021 18:50
Operator : SY/MD
Sample : M4277-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc