

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023048.D
 Acq On : 26 Oct 2021 19:14
 Operator : SY/MD
 Sample : M4277-16DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023048.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	43	50	60	rBV	310857	270058	52.00%	6.318%
2	1.304	75	82	97	rVB	79489	86563	16.67%	2.025%
3	1.568	155	164	178	rBV	52961	61337	11.81%	1.435%
4	2.108	320	332	344	rBV	113211	164325	31.64%	3.844%
5	2.185	347	356	359	rBV	5396	7877	1.52%	0.184%
6	2.507	446	456	467	rVB	15887	26389	5.08%	0.617%
7	3.912	881	893	920	rBV3	40376	152003	29.27%	3.556%
8	4.349	1012	1029	1056	rBV2	89611	230228	44.33%	5.386%
9	5.050	1227	1247	1274	rBV3	207035	519380	100.00%	12.151%
10	5.619	1410	1424	1448	rBV	150226	308371	59.37%	7.214%
11	6.072	1551	1565	1587	rBV	116481	247226	47.60%	5.784%
12	6.989	1840	1850	1878	rBV2	53315	104637	20.15%	2.448%
13	7.317	1941	1952	1971	rBV	230995	413974	79.71%	9.685%
14	7.625	2037	2048	2071	rBV2	32934	61608	11.86%	1.441%
15	8.095	2184	2194	2232	rBV	175433	430976	82.98%	10.083%
16	8.854	2419	2430	2459	rBV	232716	388316	74.77%	9.084%
17	10.217	2844	2854	2869	rBV	82015	129164	24.87%	3.022%
18	11.249	3165	3175	3197	rBV	208592	332935	64.10%	7.789%
19	11.625	3281	3292	3312	rBV	215212	339127	65.29%	7.934%




Sum of corrected areas: 4274494

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023048.D
Acq On : 26 Oct 2021 19:14
Operator : SY/MD
Sample : M4277-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

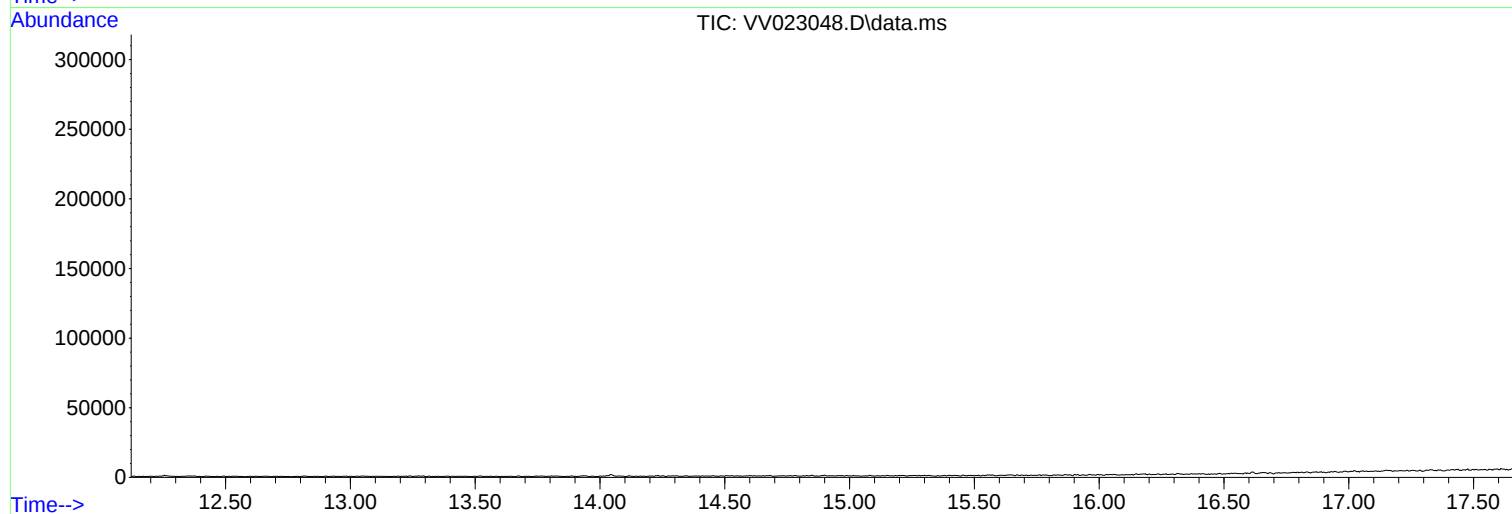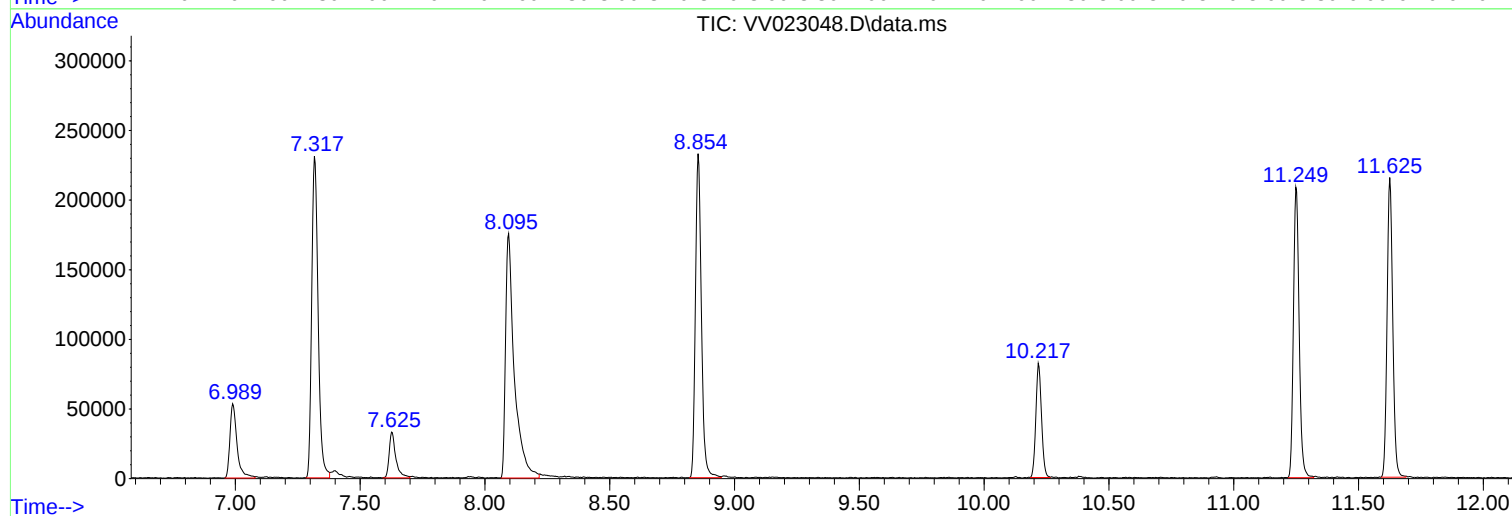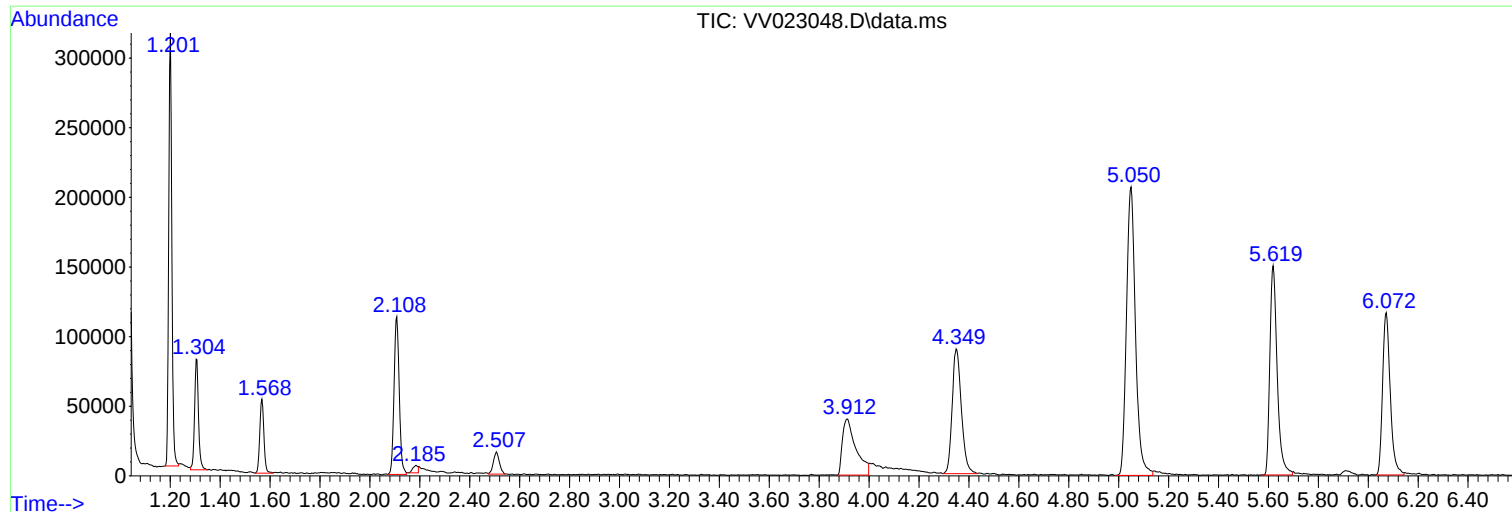

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023048.D
Acq On : 26 Oct 2021 19:14
Operator : SY/MD
Sample : M4277-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	4.38 ug/L	270058	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4
4			Cyanogen chloride	61	CClN	000506-77-4	4
5			Trifluoroguanidine	113	CH2F3N3	037950-72-4	4

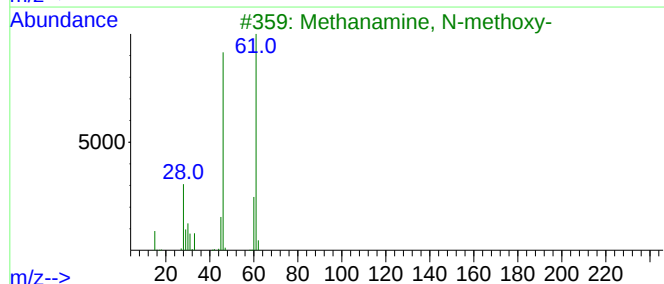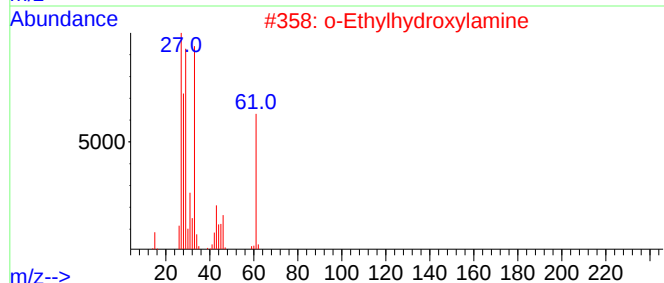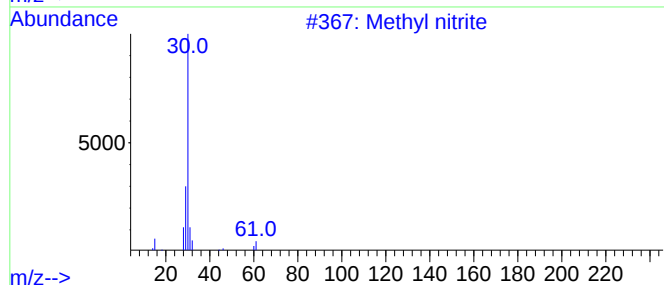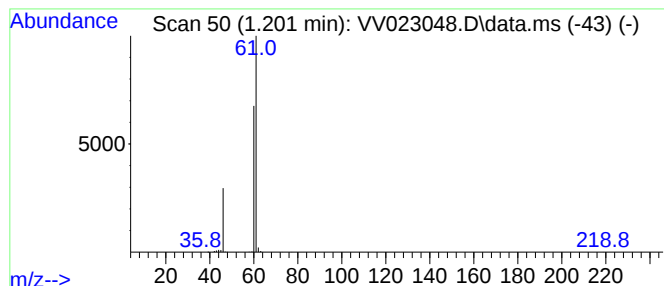

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023048.D
Acq On : 26 Oct 2021 19:14
Operator : SY/MD
Sample : M4277-16DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	4.4	ug/L	270058	1	5.619	308371	5.0