

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023049.D
 Acq On : 26 Oct 2021 19:38
 Operator : SY/MD
 Sample : M4277-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFGE1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023049.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	45	50	59	rBV4	4970	6498	1.20%	0.136%
2	1.307	76	83	97	rVB	80206	83399	15.40%	1.742%
3	1.568	153	164	176	rBV	54703	61422	11.34%	1.283%
4	2.108	321	332	342	rBV	104804	151739	28.02%	3.170%
5	2.175	342	353	381	rVB	185096	414880	76.62%	8.668%
6	2.355	383	409	410	rBV5	25948	75350	13.92%	1.574%
7	3.911	875	893	923	rBV2	178668	541461	100.00%	11.312%
8	4.352	1013	1030	1058	rBV3	76195	225205	41.59%	4.705%
9	5.050	1230	1247	1279	rBV2	200811	510154	94.22%	10.658%
10	5.619	1409	1424	1444	rBV	144872	300193	55.44%	6.272%
11	6.072	1549	1565	1591	rBV	115763	248103	45.82%	5.183%
12	6.989	1840	1850	1872	rBV	53011	101473	18.74%	2.120%
13	7.316	1940	1952	1970	rBV	233152	409560	75.64%	8.557%
14	7.397	1971	1977	1989	rVB2	7735	14570	2.69%	0.304%
15	7.625	2039	2048	2063	rBV	31085	56348	10.41%	1.177%
16	8.091	2182	2193	2233	rBV	205410	415638	76.76%	8.684%
17	8.853	2417	2430	2453	rBV	225344	376466	69.53%	7.865%
18	10.217	2843	2854	2871	rBV	78572	124902	23.07%	2.609%
19	11.249	3165	3175	3196	rBV	207873	324306	59.89%	6.775%
20	11.535	3256	3264	3274	rBV7	3591	6256	1.16%	0.131%
21	11.625	3281	3292	3309	rBV	210830	338542	62.52%	7.073%




Sum of corrected areas: 4786465

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023049.D
Acq On : 26 Oct 2021 19:38
Operator : SY/MD
Sample : M4277-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

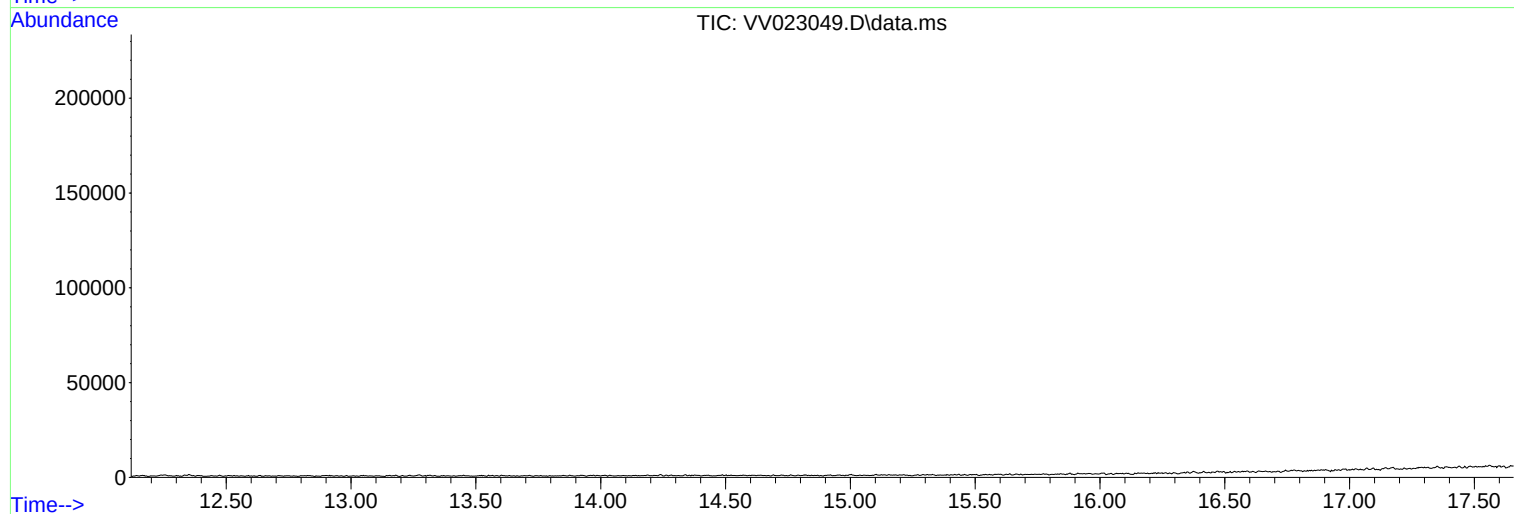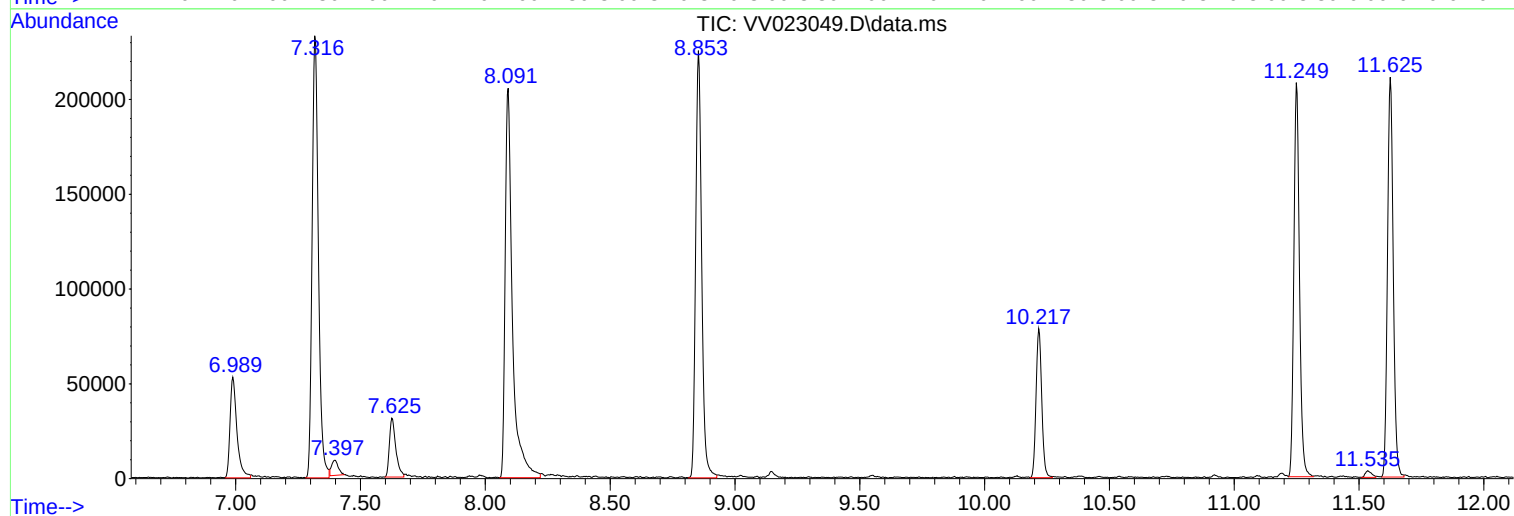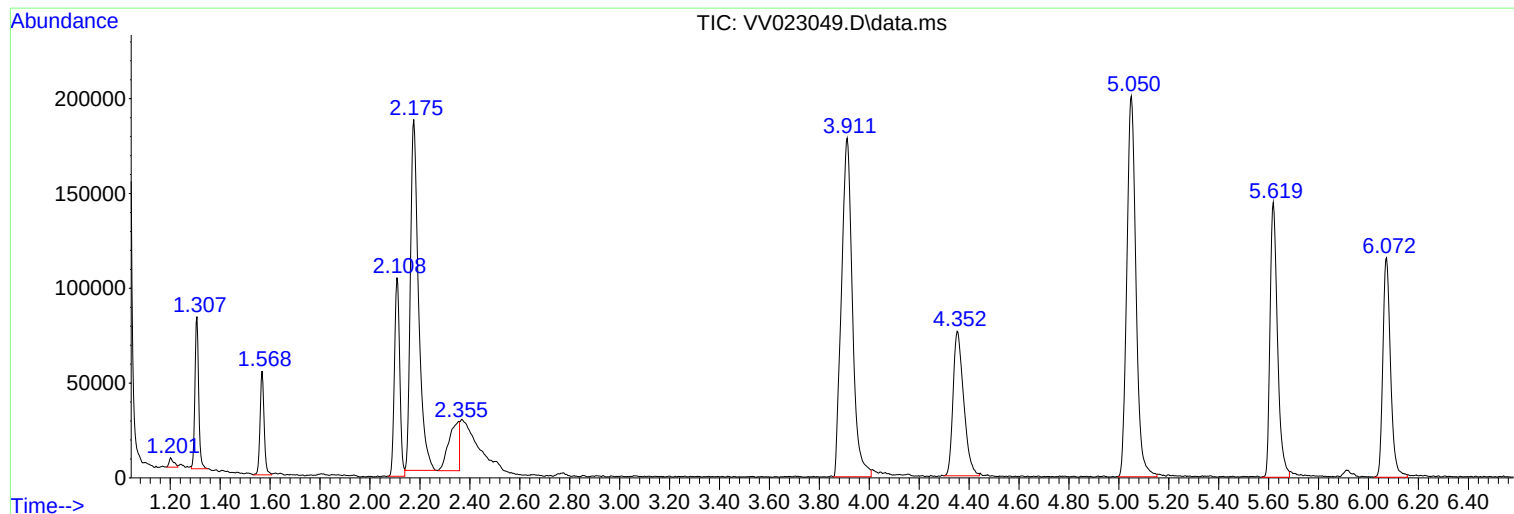

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023049.D
Acq On : 26 Oct 2021 19:38
Operator : SY/MD
Sample : M4277-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.355	1.26 ug/L	75350	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	72
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
4			Hydrazine, 1,2-dimethyl-	60	C2H8N2	000540-73-8	9
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

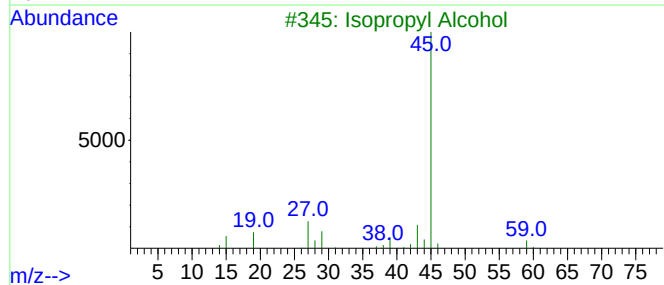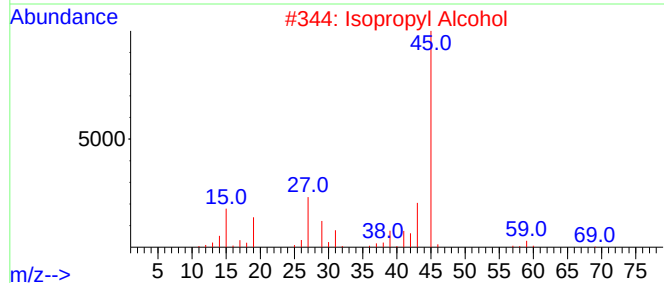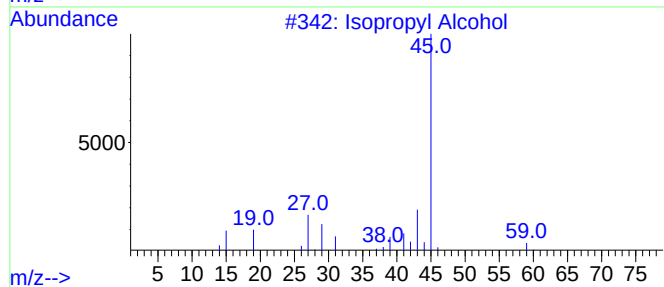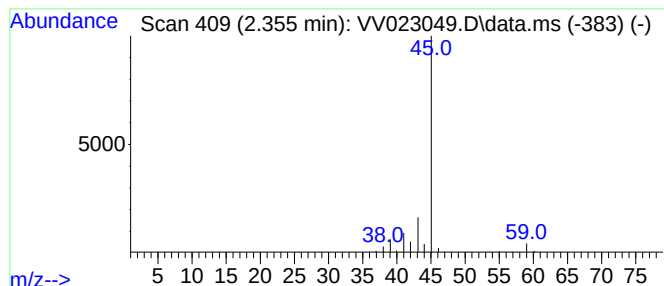

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023049.D
Acq On : 26 Oct 2021 19:38
Operator : SY/MD
Sample : M4277-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFGE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.355	1.3	ug/L	75350	1	5.619	300193	5.0