

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
 Data File : VV023050.D
 Acq On : 26 Oct 2021 20:02
 Operator : SY/MD
 Sample : M4277-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023050.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	86590	92446	16.75%	2.283%
2	1.568	156	164	174	rBV	57768	64981	11.77%	1.605%
3	2.108	320	332	350	rBV	94206	136702	24.76%	3.376%
4	2.506	441	456	468	rBV2	5761	9641	1.75%	0.238%
5	3.905	879	891	935	rBV2	28473	119572	21.66%	2.953%
6	4.355	1014	1031	1057	rBV3	62292	184558	33.43%	4.558%
7	5.050	1230	1247	1275	rBV2	218199	552022	100.00%	13.633%
8	5.619	1412	1424	1453	rBV	151137	312978	56.70%	7.729%
9	5.915	1505	1516	1528	rBV9	4328	8700	1.58%	0.215%
10	6.072	1552	1565	1588	rBV	124451	262201	47.50%	6.475%
11	6.989	1840	1850	1877	rBV2	55482	107118	19.40%	2.645%
12	7.317	1938	1952	1968	rBV	251291	441378	79.96%	10.900%
13	7.397	1974	1977	1990	rVB9	3965	6445	1.17%	0.159%
14	7.625	2039	2048	2065	rBV	33654	61709	11.18%	1.524%
15	8.091	2183	2193	2229	rBV2	212951	449651	81.46%	11.105%
16	8.853	2419	2430	2458	rBV	241762	399211	72.32%	9.859%
17	10.217	2843	2854	2874	rBV	82323	132478	24.00%	3.272%
18	11.252	3165	3176	3197	rBV	219923	343363	62.20%	8.480%
19	11.625	3280	3292	3312	rBV	232049	364073	65.95%	8.991%




Sum of corrected areas: 4049227

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023050.D
Acq On : 26 Oct 2021 20:02
Operator : SY/MD
Sample : M4277-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

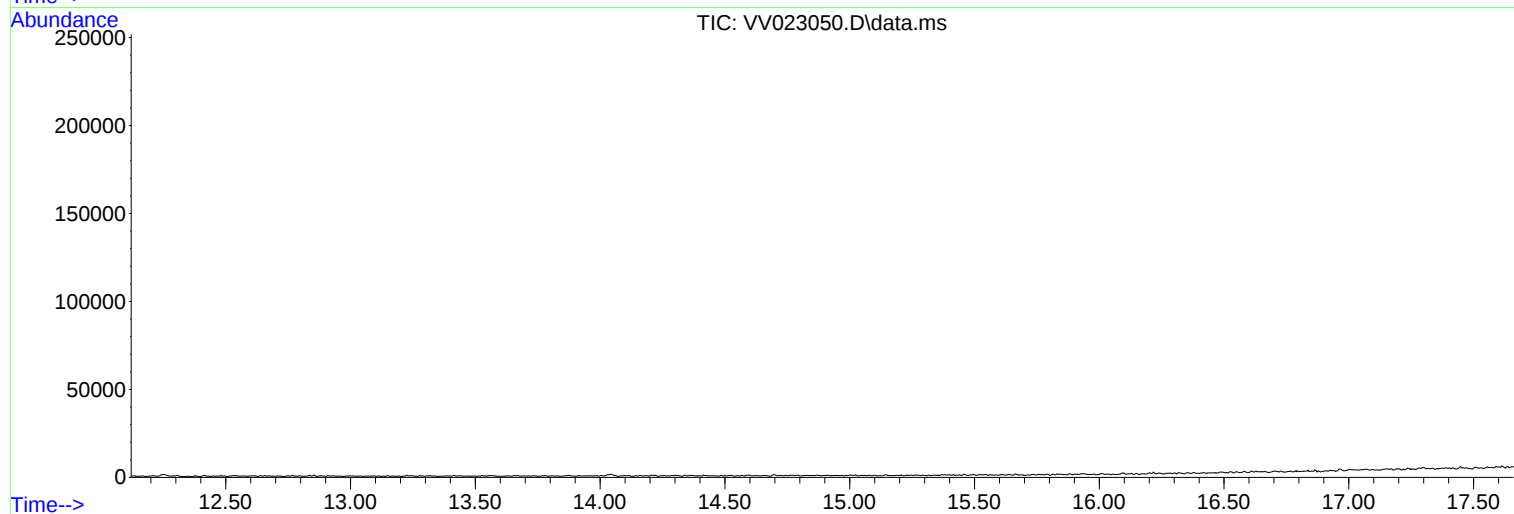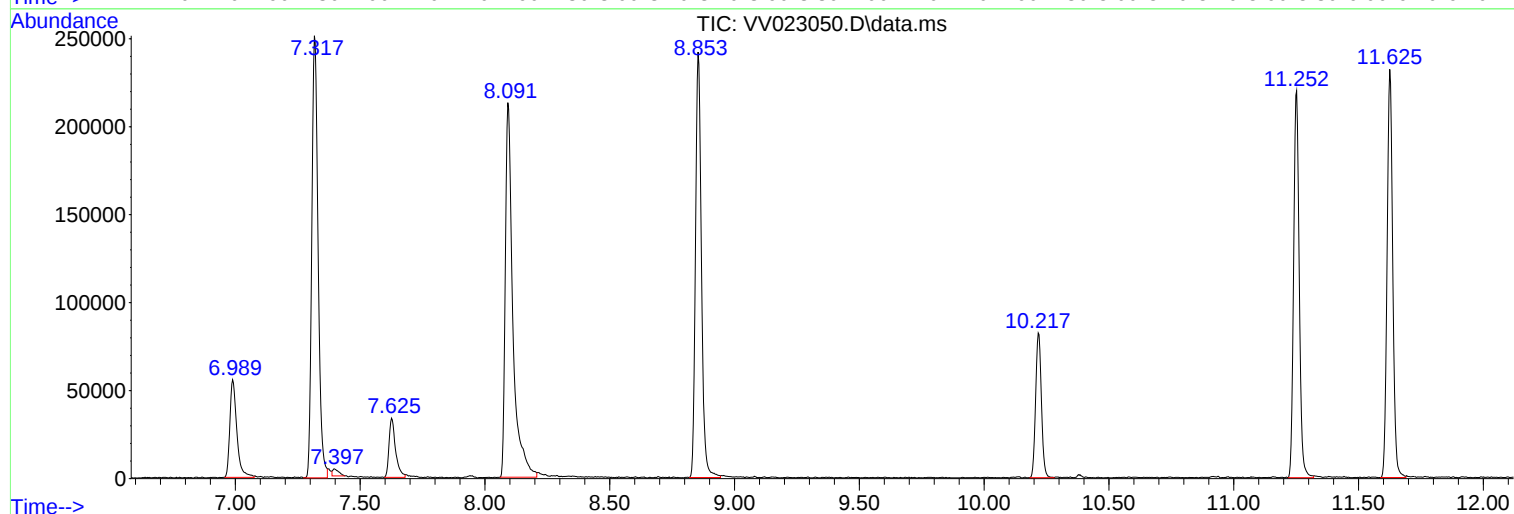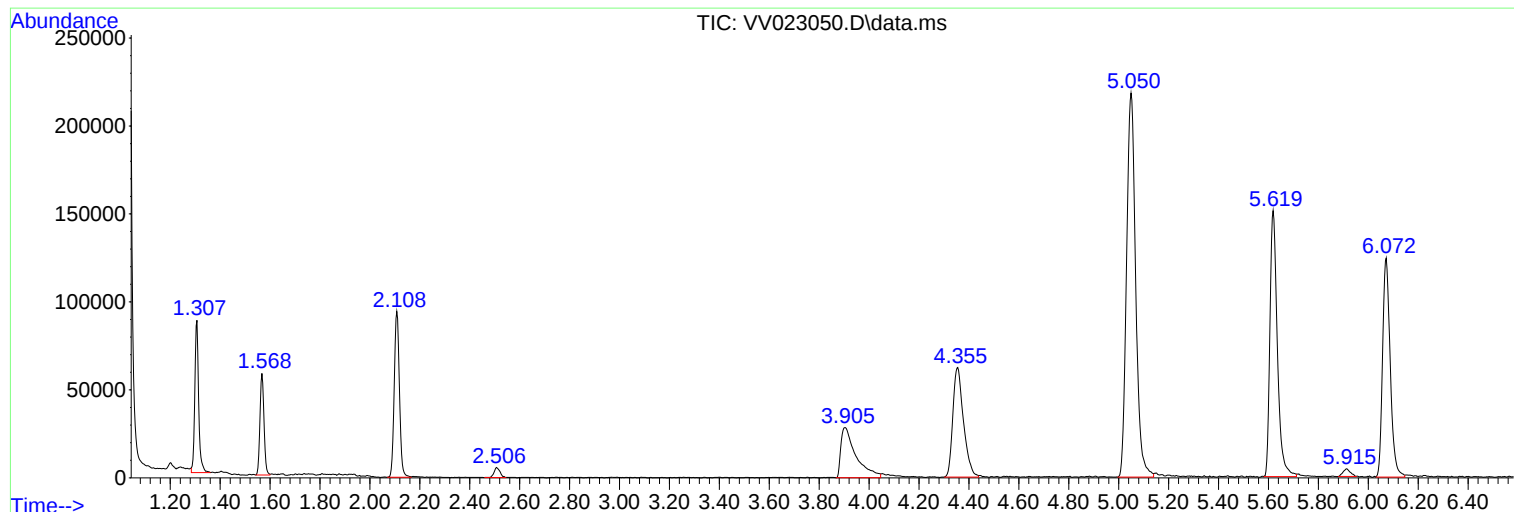

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023050.D
Acq On : 26 Oct 2021 20:02
Operator : SY/MD
Sample : M4277-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023050.D
Acq On : 26 Oct 2021 20:02
Operator : SY/MD
Sample : M4277-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc