


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102621\
Data File : VV023026.D
Acq On : 26 Oct 2021 08:41
Operator : SY/MD
Sample : BFB222
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB222

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Oct 28 01:43:46 2021

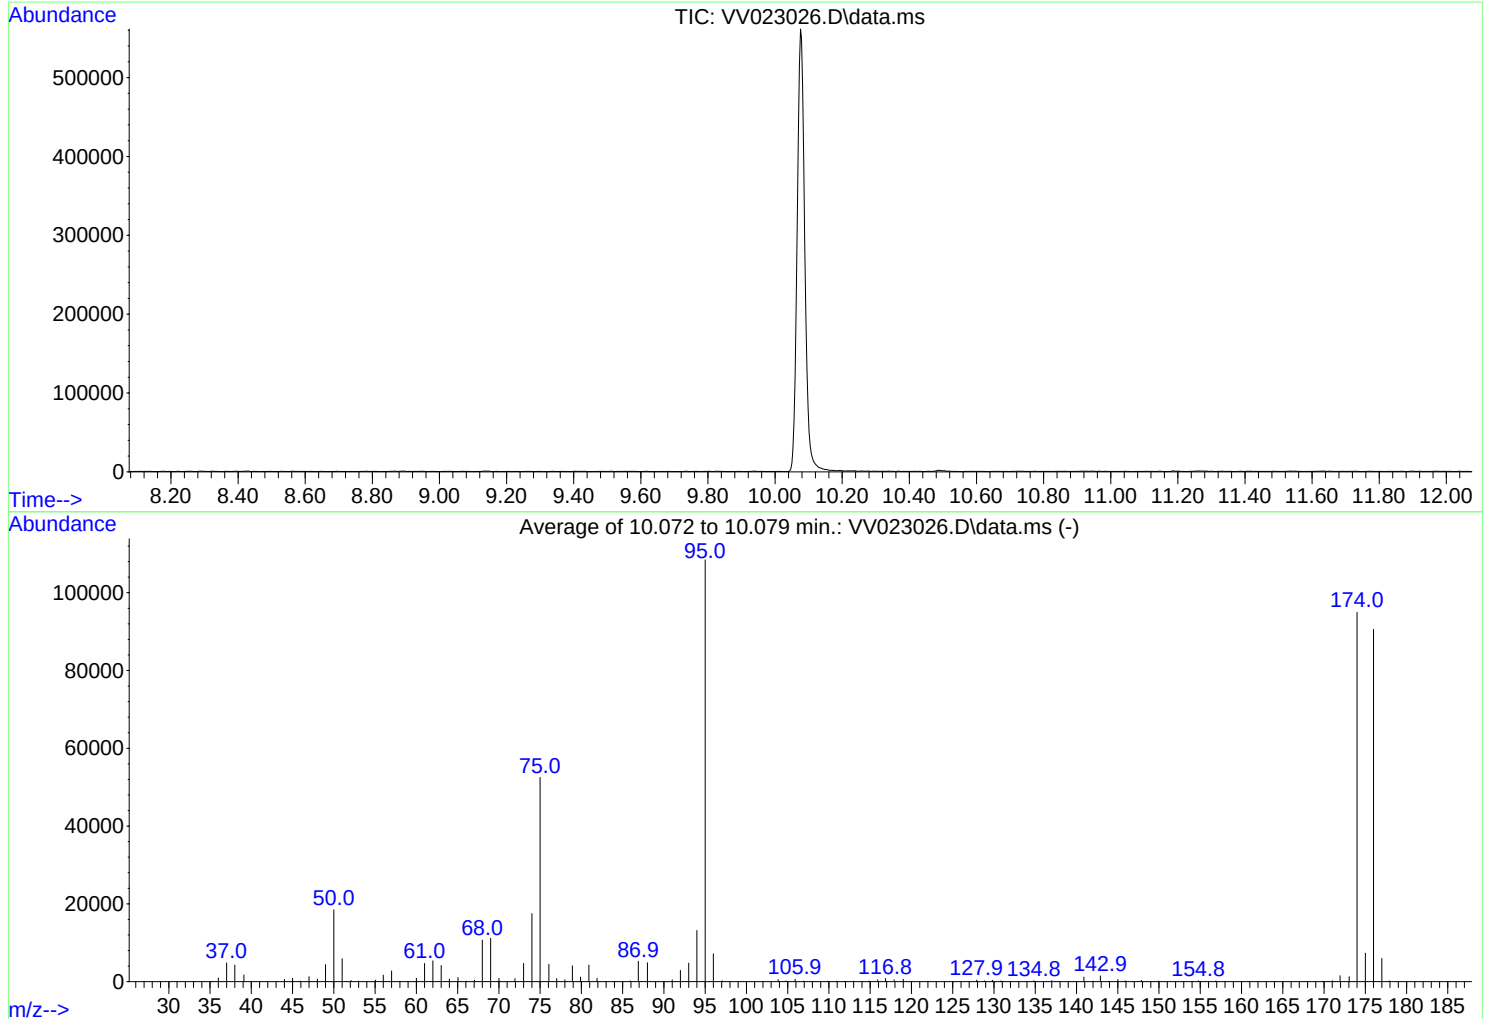

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.0	18472	PASS
75	95	30	80	48.4	52496	PASS
95	95	100	100	100.0	108453	PASS
96	95	5	9	6.6	7152	PASS
173	174	0.00	2	1.4	1288	PASS
174	95	50	120	87.6	94957	PASS
175	174	5	9	7.7	7324	PASS
176	174	95	105	95.4	90576	PASS
177	176	5	10	6.6	5950	PASS

m/z	Abundance
40.10	187.0
44.00	299.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
36.00	964.0
37.00	4762.0
38.00	4144.0
39.10	1657.0
40.00	221.0
41.10	127.0
44.00	847.0
45.00	888.0
45.90	185.0
47.00	1213.0
48.00	617.0
49.00	4257.0
50.00	17696.0
51.00	5638.0
52.10	289.0
52.90	174.0
55.10	349.0
56.00	1637.0
57.00	2762.0
58.00	136.0
60.00	889.0
61.00	4708.0
62.00	5306.0
63.00	4137.0
64.00	608.0
65.00	990.0
66.10	115.0
67.10	326.0
68.00	10476.0
69.00	10948.0
70.00	895.0
71.90	711.0
73.00	4271.0
74.00	16456.0
75.00	50632.0
76.00	4317.0
77.00	769.0
78.00	495.0
78.90	3867.0
79.90	1140.0
80.90	4189.0
81.90	902.0
85.90	189.0
86.90	4827.0
88.00	4758.0
91.00	443.0
92.00	2639.0
93.00	4646.0
94.00	12599.0
95.00	105016.0
96.00	7011.0
97.10	223.0
103.80	501.0
104.80	197.0
105.90	605.0
107.00	106.0
109.80	124.0
110.90	121.0
111.90	101.0
113.00	168.0
114.80	212.0
115.90	465.0
116.90	814.0
117.90	498.0
119.00	577.0
127.90	361.0
128.80	191.0
129.80	309.0
130.80	202.0
134.90	212.0
137.00	214.0
140.90	1088.0
142.00	167.0
142.90	1432.0
145.00	496.0
145.90	279.0
146.80	108.0
147.80	318.0
149.90	113.0
154.80	212.0
156.90	204.0
171.10	236.0
171.90	1301.0
173.10	1233.0
174.00	88064.0
175.00	6966.0
176.00	84688.0
177.00	5779.0
177.90	209.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
35.20	105.0
36.00	1009.0
37.00	5027.0
38.00	4381.0
39.10	1763.0
40.00	250.0
41.10	112.0
44.00	885.0
45.00	860.0
45.90	177.0
47.00	1290.0
48.00	690.0
49.00	4550.0
50.00	18968.0
51.00	6154.0
52.10	311.0
53.00	182.0
55.10	379.0
56.00	1721.0
57.00	2813.0
58.00	142.0
60.00	879.0
61.00	4809.0
62.00	5541.0
63.00	4298.0
64.00	720.0
65.00	1102.0
66.10	129.0
67.00	406.0
68.00	10999.0
69.00	11577.0
70.00	899.0
72.00	806.0
73.00	4862.0
74.00	18224.0
75.00	54352.0
76.00	4617.0
77.00	831.0
78.00	439.0
78.90	4256.0
79.90	1250.0
80.90	4513.0
81.90	896.0
82.90	123.0
85.90	201.0
86.90	5502.0
88.00	5034.0
91.00	483.0
92.00	2935.0
93.00	4961.0
94.00	13665.0
95.00	112368.0
96.00	7341.0
97.00	249.0
103.80	568.0
104.80	211.0
105.90	649.0
106.90	160.0
109.80	115.0
111.00	135.0
113.00	170.0
114.90	203.0
115.90	485.0
116.90	828.0
117.90	490.0
119.00	655.0
127.90	433.0
128.90	205.0
129.80	382.0
130.80	205.0
134.80	263.0
137.00	247.0
140.90	1258.0
142.00	189.0
142.90	1503.0
145.00	595.0
145.90	276.0
146.80	107.0
147.80	339.0
149.90	153.0
152.90	100.0
154.80	254.0
156.90	177.0
169.80	132.0
171.00	254.0
171.90	1595.0
173.00	1315.0
174.00	98544.0
175.00	7565.0
176.00	93376.0
177.00	6170.0
177.90	234.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

m/z	Abundance
35.20	121.0
36.00	903.0
37.00	4648.0
38.00	4220.0
39.10	1726.0
40.10	308.0
44.00	889.0
45.00	840.0
45.90	144.0
47.00	1291.0
48.00	641.0
49.00	4282.0
50.00	18752.0
51.00	5869.0
52.10	312.0
53.10	194.0
55.00	354.0
56.00	1654.0
57.00	2649.0
58.00	158.0
60.00	874.0
61.00	4589.0
62.00	5218.0
63.00	4000.0
64.00	672.0
65.10	1132.0
66.10	141.0
67.00	421.0
68.00	10578.0
69.00	10975.0
70.00	777.0
72.00	788.0
73.00	4958.0
74.00	17744.0
75.00	52504.0
76.10	4439.0
77.00	791.0
78.00	428.0
78.90	4133.0
79.90	1242.0
80.90	4155.0
81.90	851.0
82.90	166.0
85.90	192.0
86.90	5329.0
88.00	4810.0
91.00	498.0
92.00	3124.0
93.00	4765.0
94.00	13189.0
95.00	107976.0
96.00	7105.0
97.00	282.0
103.90	591.0
104.80	236.0
105.90	617.0
106.90	211.0
108.00	126.0
110.90	145.0
112.90	133.0
114.90	144.0
115.90	507.0
116.80	828.0
117.90	440.0
119.00	676.0
127.90	459.0
128.90	188.0
129.80	422.0
130.90	223.0
134.80	270.0
137.00	256.0
140.90	1300.0
142.00	177.0
142.90	1532.0
143.90	109.0
145.00	564.0
145.90	237.0
146.70	105.0
147.90	305.0
149.90	177.0
152.90	102.0
154.80	286.0
156.90	203.0
157.90	108.0
160.90	118.0
169.80	162.0
171.00	239.0
172.00	1629.0
173.00	1317.0
174.00	98264.0
175.00	7442.0
176.00	93664.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222

177.005901.0

177.90206.0

Instrument :
MSVOA_V
ClientSampleId :
BFB222