

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
 Data File : VV028697.D
 Acq On : 26 Oct 2022 15:59
 Operator : SY/MD
 Sample : N5216-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA79

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	95	rBV	79306	81461	13.56%	1.591%
2	1.449	122	127	135	rVB10	6684	8464	1.41%	0.165%
3	1.564	156	163	175	rBV	78681	91802	15.28%	1.793%
4	2.105	320	331	346	rBV	141484	204290	34.01%	3.990%
5	2.764	522	536	551	rBV	30753	66946	11.15%	1.308%
6	3.892	876	887	929	rBV	72692	273821	45.59%	5.349%
7	4.352	1014	1030	1056	rBV3	110878	379616	63.21%	7.415%
8	5.043	1231	1245	1271	rBV2	216854	551805	91.87%	10.779%
9	5.616	1408	1423	1443	rBV	206276	425695	70.88%	8.315%
10	6.069	1552	1564	1586	rBV	132155	280061	46.63%	5.471%
11	6.580	1709	1723	1732	rBV	6834	17203	2.86%	0.336%
12	6.989	1840	1850	1862	rBV2	48663	92626	15.42%	1.809%
13	7.133	1887	1895	1909	rVB5	10610	22791	3.79%	0.445%
14	7.313	1938	1951	1974	rBV	236845	432775	72.06%	8.454%
15	7.625	2039	2048	2061	rBV2	25574	44707	7.44%	0.873%
16	8.088	2182	2192	2229	rBV2	258379	600605	100.00%	11.732%
17	8.847	2418	2428	2447	rBV	316383	539995	89.91%	10.548%
18	10.210	2842	2852	2870	rBV	89161	148286	24.69%	2.897%
19	10.378	2892	2904	2911	rBV9	4793	7848	1.31%	0.153%
20	11.242	3161	3173	3191	rBV	299462	491604	81.85%	9.603%
21	11.619	3277	3290	3308	rBV	214773	357016	59.44%	6.974%




Sum of corrected areas: 5119417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
Data File : VV028697.D
Acq On : 26 Oct 2022 15:59
Operator : SY/MD
Sample : N5216-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

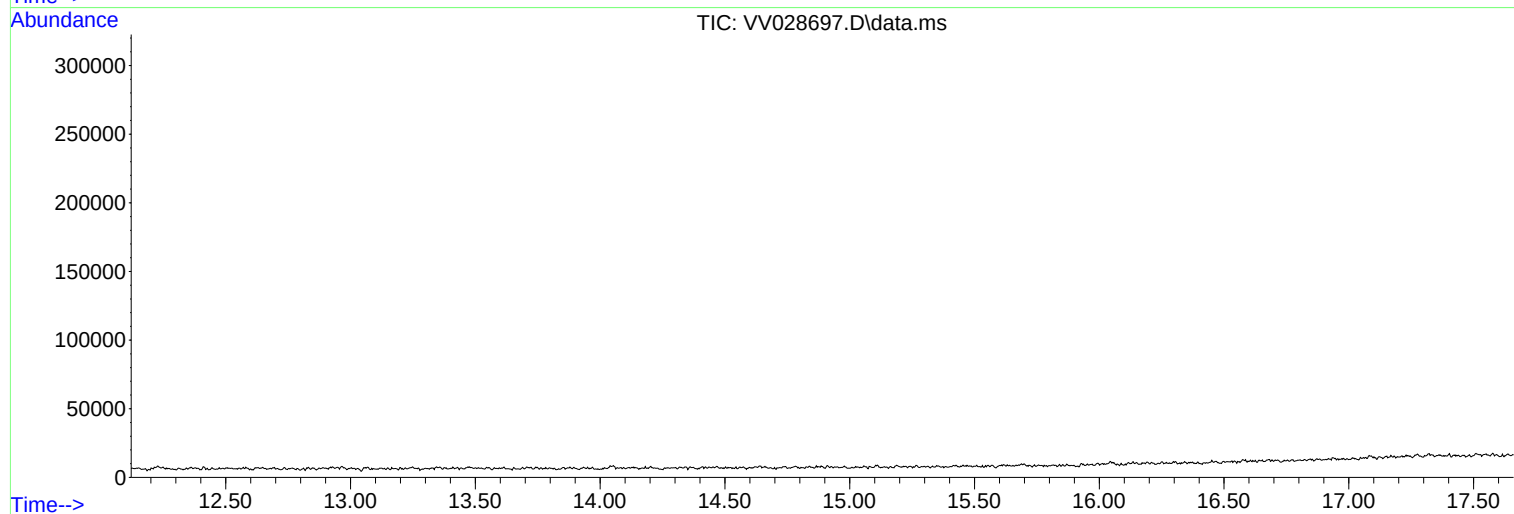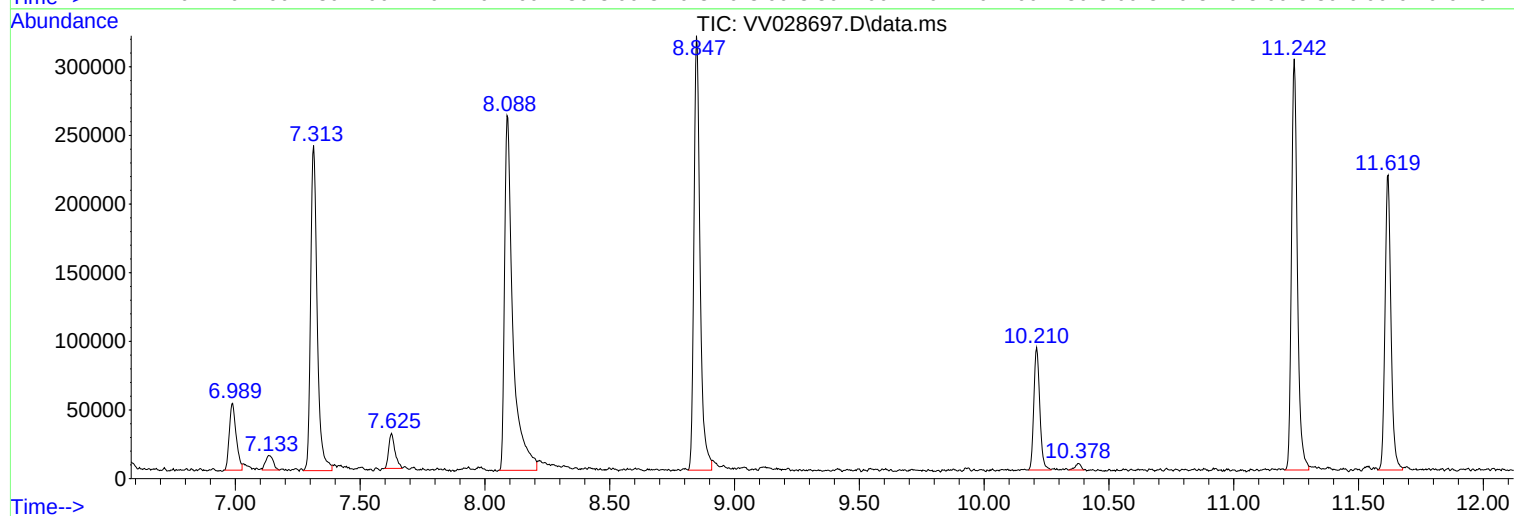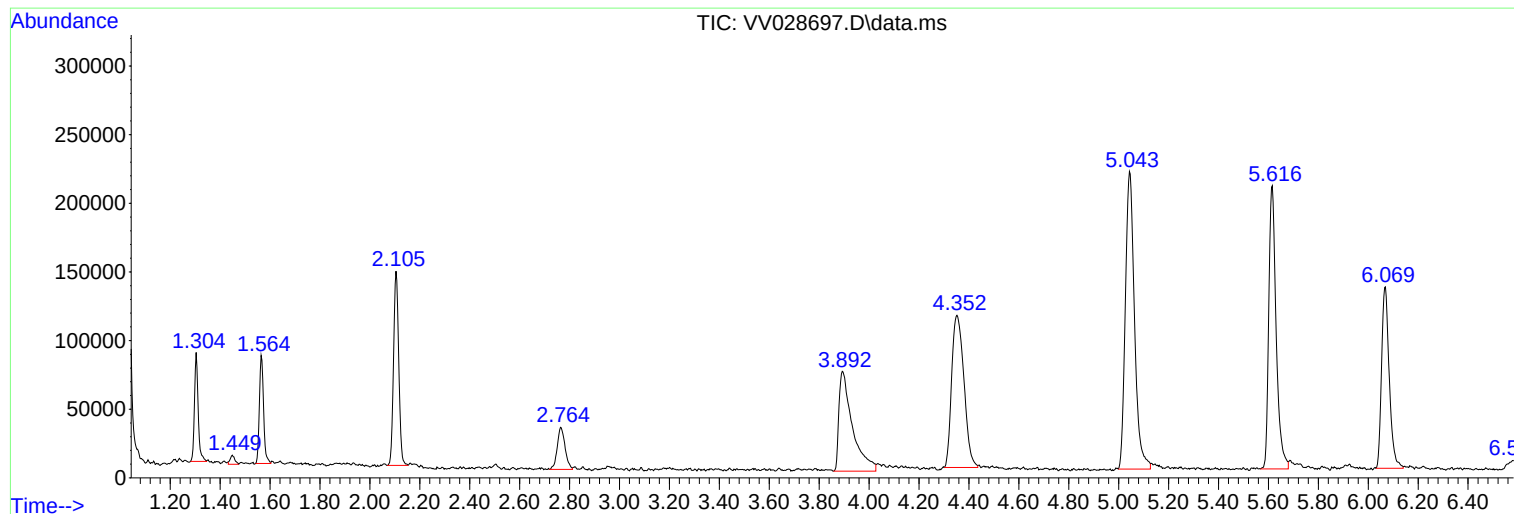

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
Data File : VV028697.D
Acq On : 26 Oct 2022 15:59
Operator : SY/MD
Sample : N5216-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
Data File : VV028697.D
Acq On : 26 Oct 2022 15:59
Operator : SY/MD
Sample : N5216-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc