

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
 Data File : VV028706.D
 Acq On : 26 Oct 2022 20:05
 Operator : SY/MD
 Sample : N5216-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BHA95

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV028706.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	99	rVB	79624	91071	12.99%	1.579%
2	1.449	122	127	132	rBV3	9202	10910	1.56%	0.189%
3	1.564	157	163	173	rBV	82721	95771	13.66%	1.661%
4	2.105	322	331	344	rVB	156435	230542	32.88%	3.997%
5	2.175	350	353	364	rVB3	9644	15080	2.15%	0.261%
6	3.896	876	888	922	rBV2	81108	293248	41.83%	5.085%
7	4.352	1014	1030	1056	rBV4	126066	426245	60.80%	7.391%
8	5.043	1231	1245	1277	rBV3	234906	627704	89.54%	10.884%
9	5.613	1411	1422	1447	rBV	225454	470062	67.05%	8.150%
10	6.066	1549	1563	1586	rBV2	143921	305903	43.63%	5.304%
11	6.985	1838	1849	1870	rBV	56411	118042	16.84%	2.047%
12	7.313	1937	1951	1968	rBV	255832	462344	65.95%	8.017%
13	7.394	1968	1976	1988	rVB	14985	31258	4.46%	0.542%
14	7.622	2040	2047	2061	rBV2	28864	53216	7.59%	0.923%
15	8.088	2182	2192	2233	rBV	322981	701066	100.00%	12.156%
16	8.847	2416	2428	2463	rBV	346063	657972	93.85%	11.409%
17	9.140	2509	2519	2531	rBV	11809	23215	3.31%	0.403%
18	9.542	2635	2644	2648	rBV10	6066	8550	1.22%	0.148%
19	9.931	2755	2765	2774	rBV7	6041	11702	1.67%	0.203%
20	10.210	2842	2852	2865	rBV	101209	159813	22.80%	2.771%
21	10.371	2890	2902	2904	rBV9	5482	8973	1.28%	0.156%
22	11.243	3161	3173	3191	rBV	332515	528042	75.32%	9.156%
23	11.532	3254	3263	3272	rBV	6760	12577	1.79%	0.218%
24	11.616	3279	3289	3311	rVB	233356	386662	55.15%	6.704%
25	12.342	3506	3515	3523	rBV	9435	17422	2.49%	0.302%
26	13.500	3868	3875	3884	rBV3	10246	19898	2.84%	0.345%




Sum of corrected areas: 5767288

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
Data File : VV028706.D
Acq On : 26 Oct 2022 20:05
Operator : SY/MD
Sample : N5216-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

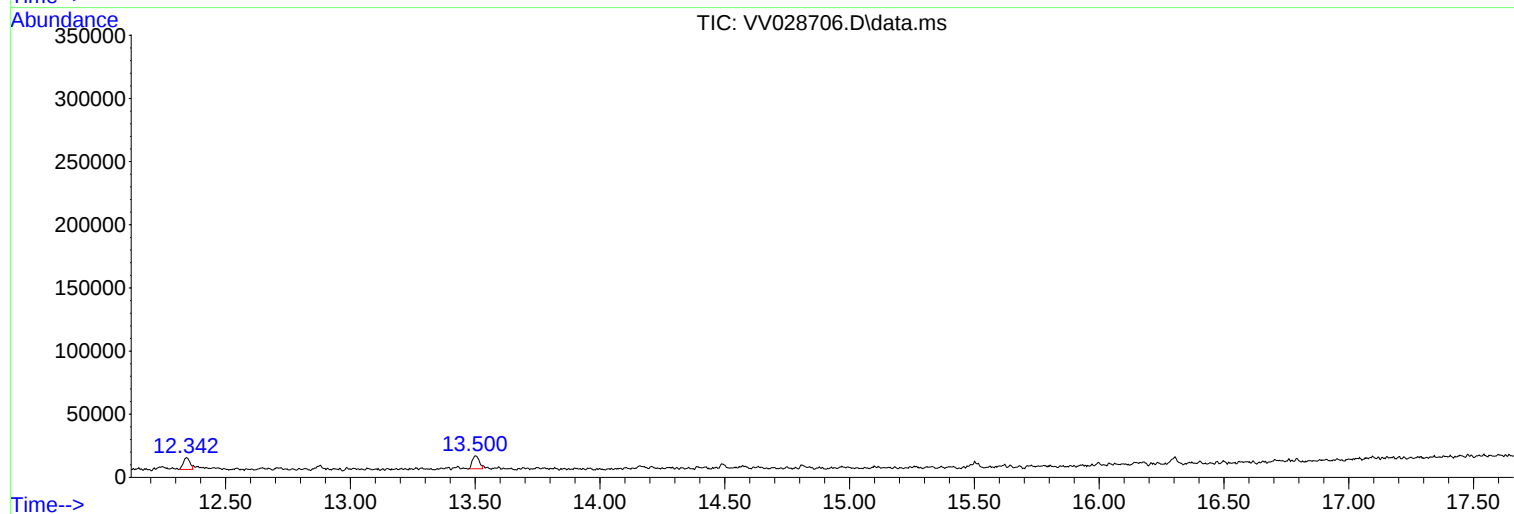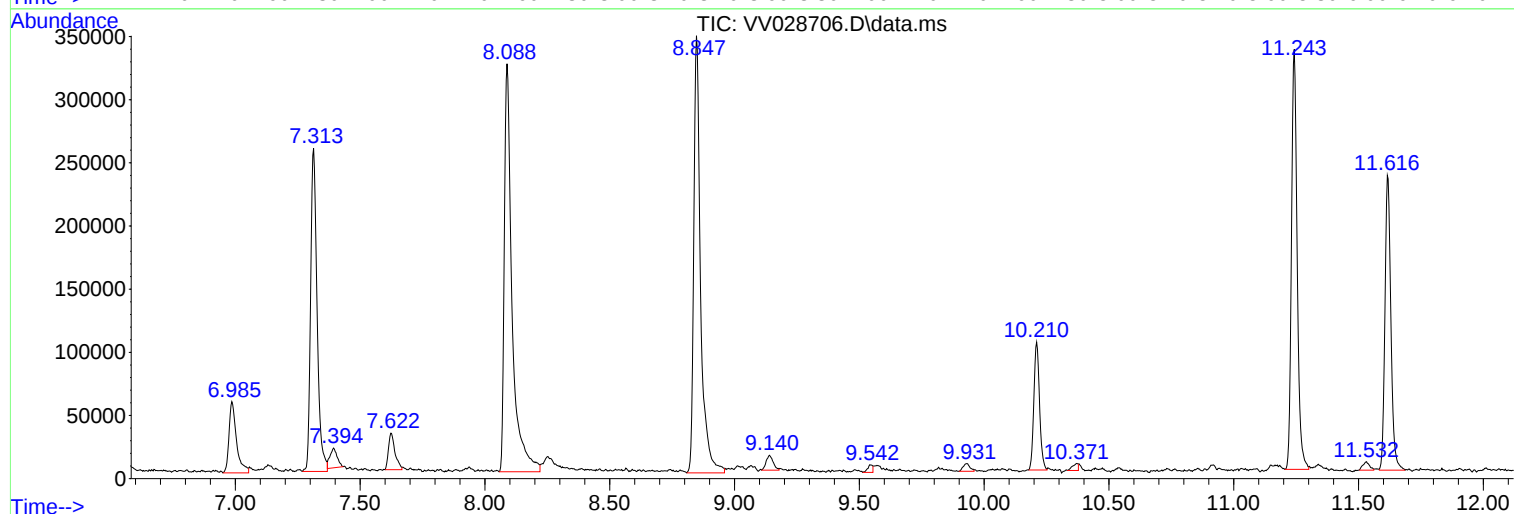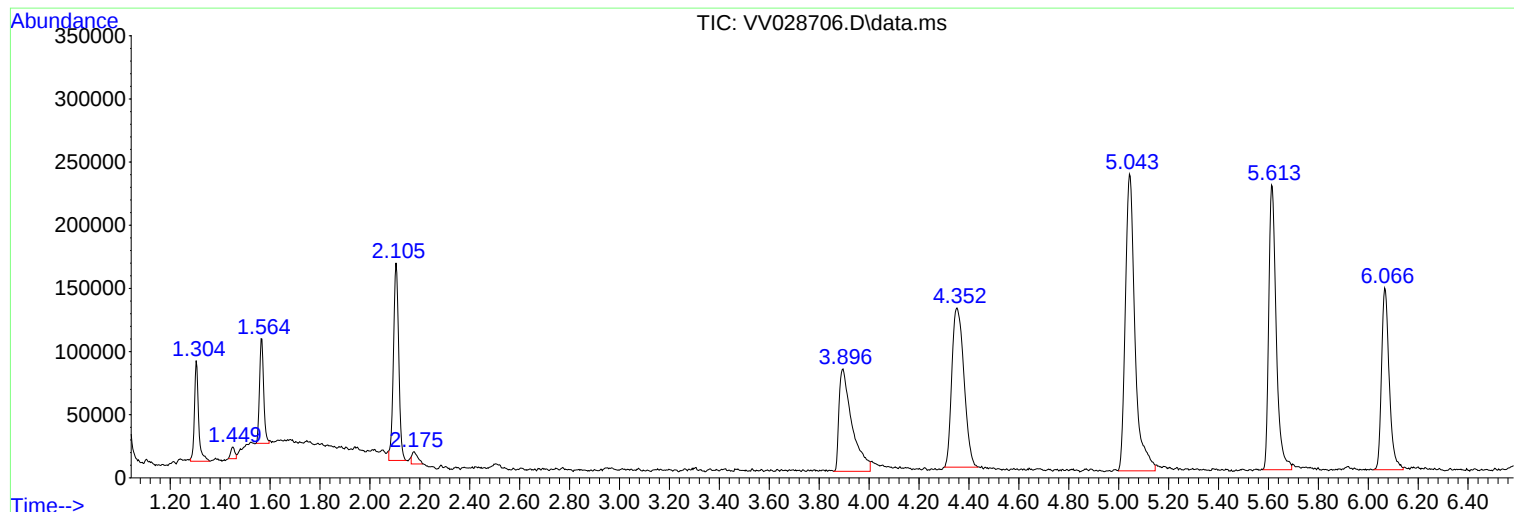

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
Data File : VV028706.D
Acq On : 26 Oct 2022 20:05
Operator : SY/MD
Sample : N5216-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
Data File : VV028706.D
Acq On : 26 Oct 2022 20:05
Operator : SY/MD
Sample : N5216-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BHA95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc