


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102622\
Data File : VV028687.D
Acq On : 26 Oct 2022 09:22
Operator : SY/MD
Sample : BFB391
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB391

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102522WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 28 21:50:06 2022

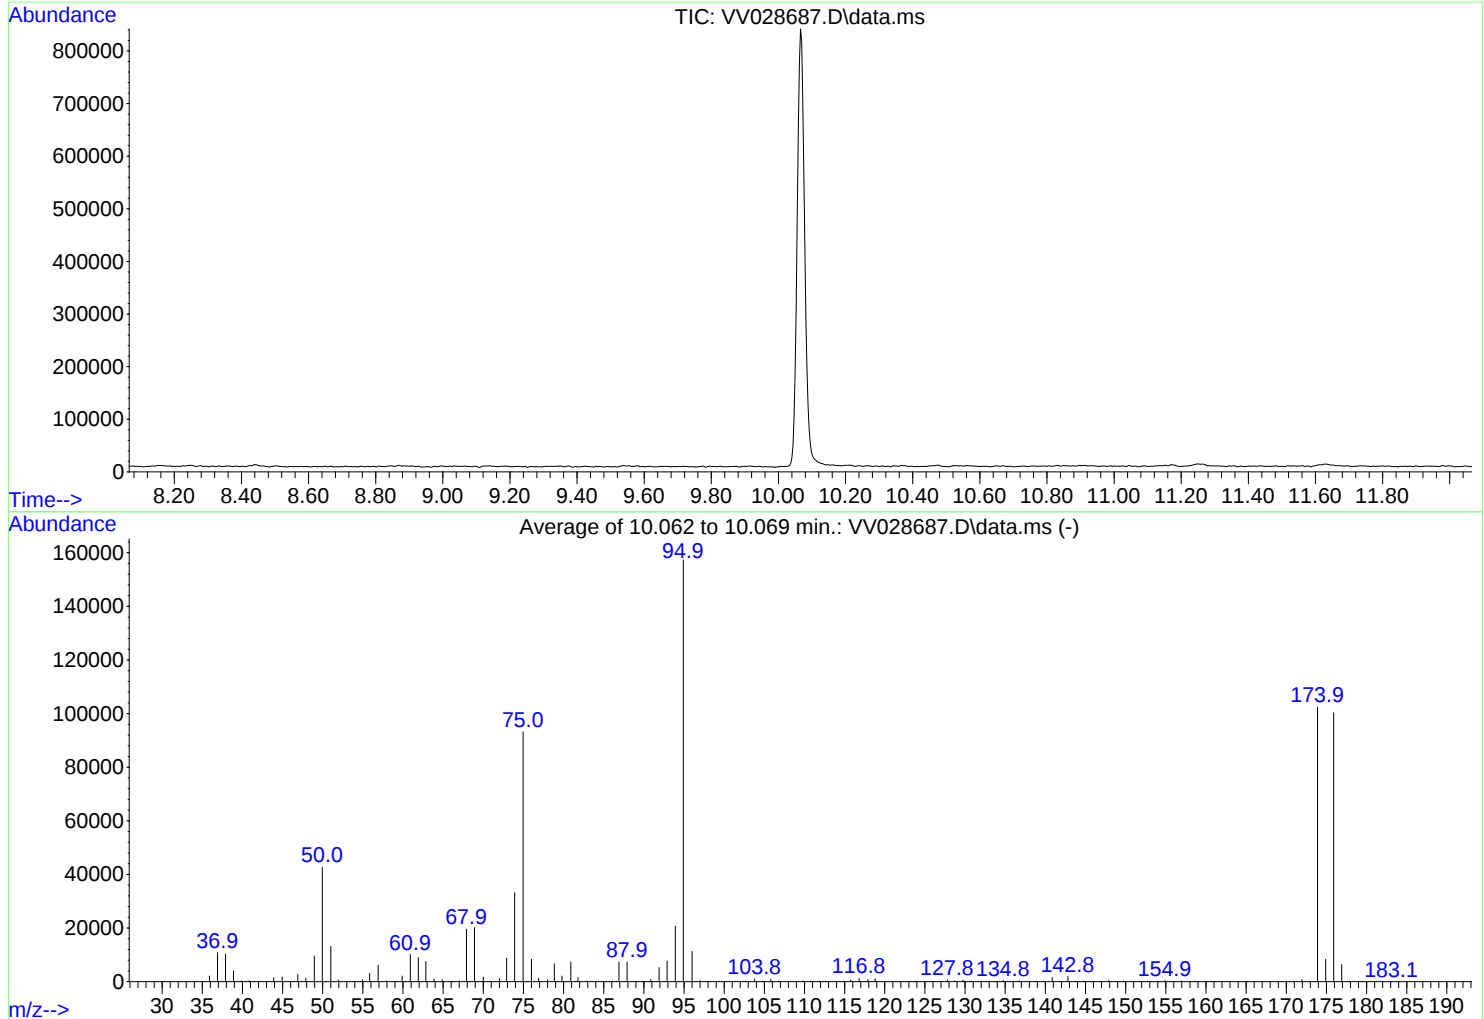

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2791

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	27.1	42695	PASS
75	95	30	80	59.2	93152	PASS
95	95	100	100	100.0	157355	PASS
96	95	5	9	7.2	11282	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	65.1	102435	PASS
175	174	5	9	8.2	8379	PASS
176	174	95	105	97.9	100317	PASS
177	176	5	10	6.3	6365	PASS

m/z	Abundance
35.80	248.0
36.90	196.0
38.80	315.0
39.90	1028.0
41.10	301.0
41.90	274.0
42.80	264.0
43.10	260.0
43.90	2880.0
44.80	520.0
45.60	210.0
46.20	213.0
46.90	173.0
47.90	130.0
49.90	129.0
50.60	154.0
51.90	135.0
52.90	218.0
54.60	181.0
55.80	153.0
57.00	186.0
58.20	110.0
59.30	142.0
60.90	131.0
62.00	176.0
62.70	113.0
67.10	125.0
68.40	139.0
72.00	111.0
76.80	292.0
78.00	112.0
79.00	148.0
81.40	104.0
115.60	104.0
171.30	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.90	2267.0
37.00	10826.0
37.90	9995.0
38.90	4031.0
39.90	1294.0
40.80	379.0
41.50	145.0
42.10	219.0
42.90	452.0
43.90	4256.0
45.00	2205.0
45.80	423.0
47.00	2887.0
47.90	1351.0
48.90	9339.0
50.00	41528.0
51.00	12817.0
52.00	745.0
52.90	297.0
53.70	158.0
54.90	727.0
55.90	3267.0
56.90	6377.0
57.90	374.0
59.10	105.0
59.90	2166.0
60.90	10064.0
61.90	8948.0
62.90	7195.0
63.90	1028.0
64.90	678.0
65.90	176.0
66.90	483.0
67.90	19104.0
68.90	19888.0
70.00	1733.0
70.90	206.0
72.00	1221.0
72.90	8300.0
73.90	31712.0
75.00	91032.0
76.00	8264.0
77.00	1598.0
78.00	695.0
78.80	6570.0
79.80	2021.0
80.90	7039.0
81.80	1517.0
82.80	311.0
84.10	158.0
85.00	126.0
85.70	194.0
86.90	7156.0
87.90	6830.0
89.80	165.0
90.80	774.0
91.90	4977.0
92.90	7365.0
93.90	19704.0
94.90	150976.0
96.00	11051.0
97.00	364.0
102.70	172.0
103.80	981.0
104.80	272.0
105.80	960.0
106.80	208.0
109.80	254.0
110.70	221.0
111.90	147.0
112.60	221.0
114.90	215.0
115.80	698.0
116.80	1164.0
117.90	706.0
118.80	985.0
122.60	101.0
123.70	160.0
125.70	137.0
127.80	651.0
128.70	353.0
129.80	638.0
130.60	213.0
131.80	108.0
133.80	132.0
134.70	419.0
136.70	302.0
138.90	158.0
139.80	157.0
140.90	1526.0
141.80	221.0
142.80	1778.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

143.80	175.0
144.80	270.0
145.60	243.0
147.00	105.0
147.90	412.0
148.80	104.0
149.70	197.0
151.90	170.0
152.70	188.0
154.90	369.0
157.00	329.0
158.70	168.0
160.70	157.0
161.10	142.0
170.10	149.0
170.90	156.0
171.90	722.0
173.90	95992.0
174.90	8076.0
175.90	92800.0
176.90	6194.0
177.90	222.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
36.00	2493.0
36.90	11258.0
37.90	10664.0
39.00	4596.0
39.90	1333.0
40.90	344.0
42.00	238.0
42.90	462.0
43.90	4361.0
45.00	2404.0
45.80	371.0
46.90	3092.0
47.90	1493.0
48.90	9915.0
50.00	44568.0
51.00	13699.0
52.00	709.0
52.90	275.0
53.80	135.0
55.00	692.0
55.90	3481.0
56.90	6551.0
57.90	369.0
59.00	107.0
59.90	2140.0
60.90	10561.0
61.90	9444.0
62.90	7860.0
63.90	1058.0
64.90	714.0
66.20	195.0
67.00	534.0
67.90	20336.0
68.90	20776.0
70.00	1788.0
71.00	199.0
72.00	1309.0
72.90	9136.0
73.90	34432.0
74.90	96488.0
76.00	8697.0
76.90	1622.0
78.00	805.0
78.80	7017.0
79.80	2159.0
80.90	7562.0
81.80	1604.0
82.90	301.0
84.10	129.0
85.10	131.0
85.70	181.0
86.10	225.0
86.90	7551.0
87.90	7642.0
89.80	168.0
90.80	854.0
91.90	5424.0
92.90	7884.0
93.90	21472.0
94.90	162752.0
96.00	11674.0
97.00	442.0
98.00	102.0
102.70	166.0
103.80	1027.0
104.80	266.0
105.80	964.0
106.80	229.0
109.80	333.0
110.80	247.0
111.90	178.0
112.60	261.0
114.80	200.0
115.80	708.0
116.80	1263.0
117.90	793.0
118.80	1160.0
123.80	173.0
125.80	140.0
127.80	703.0
128.70	424.0
129.80	647.0
130.80	246.0
131.70	103.0
133.80	135.0
134.70	403.0
136.80	299.0
138.80	159.0
139.80	160.0
140.80	1662.0
141.80	188.0
142.80	2034.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

143.80	144.0
144.80	268.0
145.80	214.0
146.80	143.0
147.90	457.0
148.80	114.0
149.70	246.0
151.80	166.0
152.70	245.0
154.90	391.0
156.90	318.0
158.60	173.0
160.70	171.0
170.00	141.0
171.00	196.0
171.90	713.0
173.90	105936.0
174.90	8630.0
175.90	103928.0
176.90	6572.0
177.90	231.0
183.10	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

m/z	Abundance
35.90	2323.0
36.90	10818.0
37.90	10200.0
39.00	4413.0
39.90	1376.0
40.90	332.0
41.90	270.0
43.00	489.0
43.90	4451.0
45.00	2413.0
46.00	354.0
46.90	2747.0
47.90	1539.0
49.00	9478.0
50.00	42376.0
51.00	12973.0
52.00	678.0
52.80	217.0
53.90	156.0
54.90	659.0
55.90	3272.0
56.90	6020.0
57.90	349.0
58.70	111.0
59.90	1933.0
60.90	10002.0
61.90	9195.0
62.90	7801.0
63.80	895.0
64.90	721.0
66.10	227.0
67.10	488.0
67.90	19376.0
68.90	19832.0
70.00	1636.0
70.90	203.0
72.00	1218.0
72.90	8831.0
73.90	33352.0
74.90	91936.0
76.00	8174.0
76.90	1393.0
78.00	798.0
78.90	6845.0
79.80	2130.0
80.90	7285.0
81.80	1619.0
83.00	292.0
85.70	201.0
86.10	281.0
86.90	7341.0
87.90	7649.0
89.70	109.0
90.90	792.0
91.90	5349.0
92.90	7638.0
93.90	21136.0
94.90	158336.0
96.00	11121.0
97.00	433.0
98.00	182.0
102.70	137.0
103.80	945.0
104.80	236.0
105.80	852.0
106.80	248.0
109.80	343.0
110.80	285.0
111.90	208.0
112.70	243.0
114.80	213.0
115.80	673.0
116.80	1200.0
117.90	757.0
118.80	1263.0
123.80	164.0
125.90	129.0
127.80	668.0
128.70	393.0
129.70	582.0
130.80	249.0
134.00	119.0
134.80	359.0
136.80	315.0
138.80	140.0
139.70	150.0
140.80	1524.0
142.80	2068.0
143.80	136.0
144.80	261.0
145.90	213.0
146.80	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391

147.90	508.0
148.80	107.0
149.70	233.0
151.70	142.0
152.70	209.0
153.90	128.0
154.90	432.0
156.80	261.0
158.60	195.0
160.70	191.0
171.00	203.0
172.00	681.0
173.90	105376.0
174.90	8431.0
175.90	104224.0
176.90	6330.0
177.80	238.0

Instrument :
MSVOA_V
ClientSampleId :
BFB391