




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032656.D
Acq On : 26 Oct 2023 12:41
Operator : SY/MD
Sample : 04995-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49K6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/27/2023
Supervised By :Mahesh Dadoda 10/27/2023

Quant Time: Oct 27 05:34:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 27 05:30:38 2023
Response via : Initial Calibration

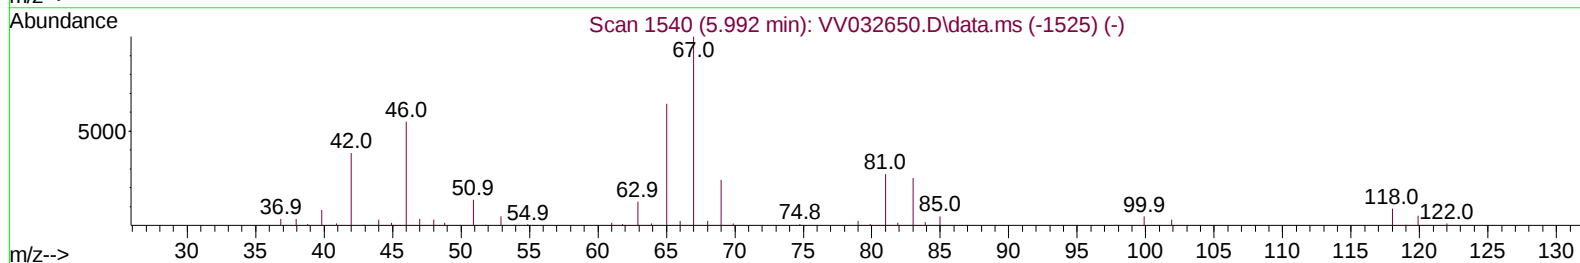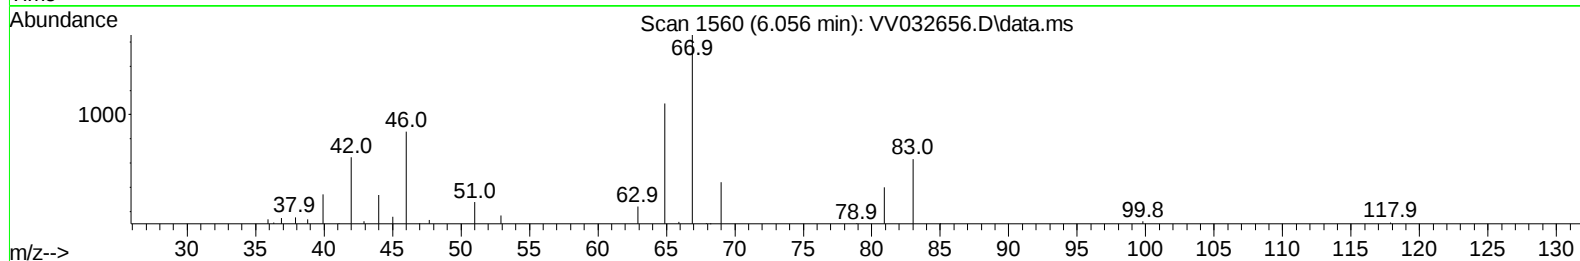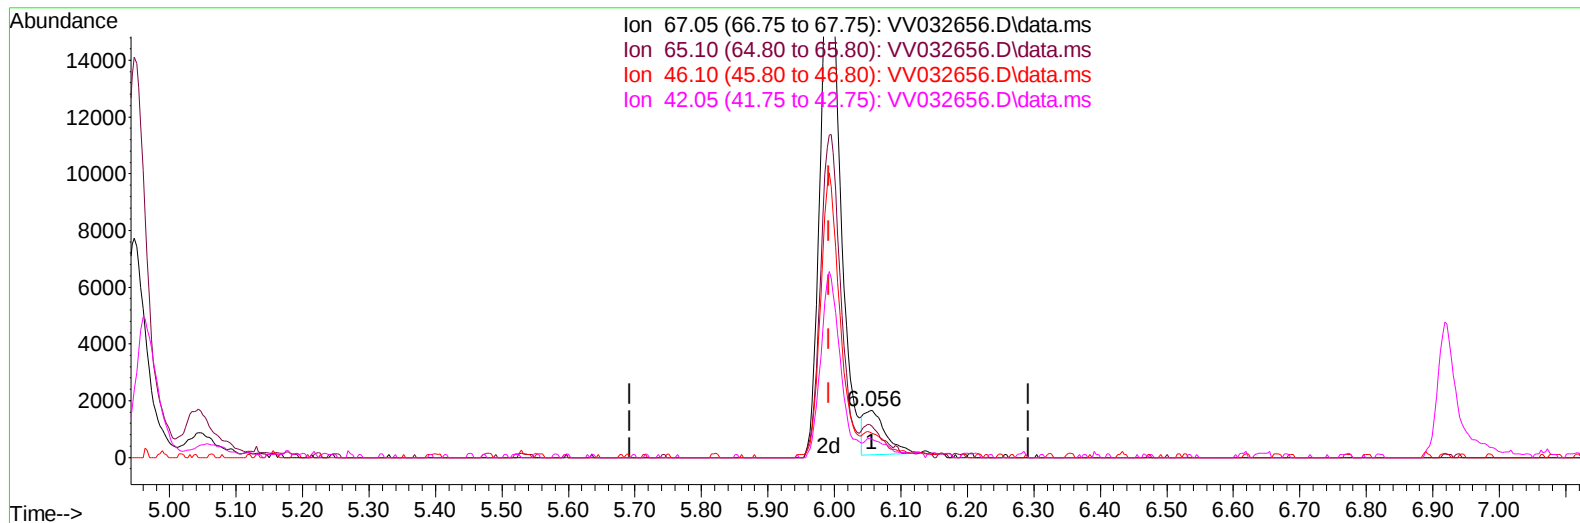

TIC: VV032656.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

6.056min (+ 0.064) 0.37 ug/L

response 3587

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	67.60	62.53
46.10	49.60	39.92
42.05	26.30	31.75




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032656.D
Acq On : 26 Oct 2023 12:41
Operator : SY/MD
Sample : 04995-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49K6

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 10/27/2023
Supervised By :Mahesh Dadoda 10/27/2023

Quant Time: Oct 27 05:34:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 27 05:30:38 2023
Response via : Initial Calibration

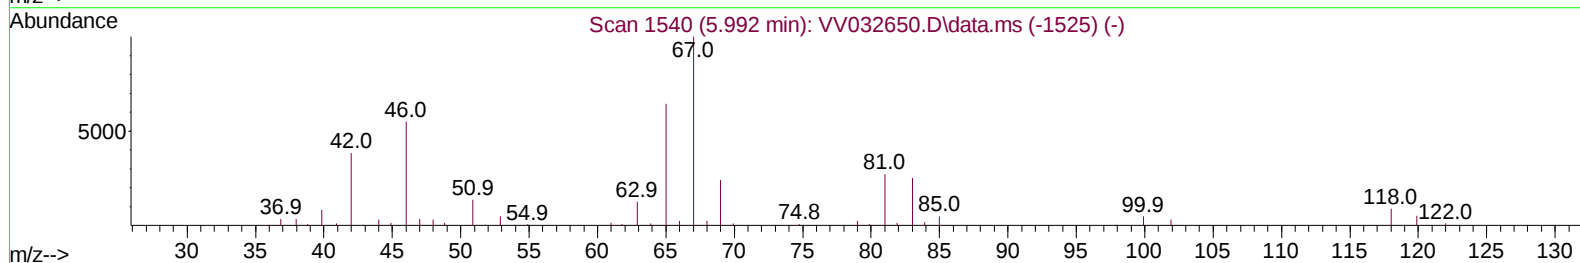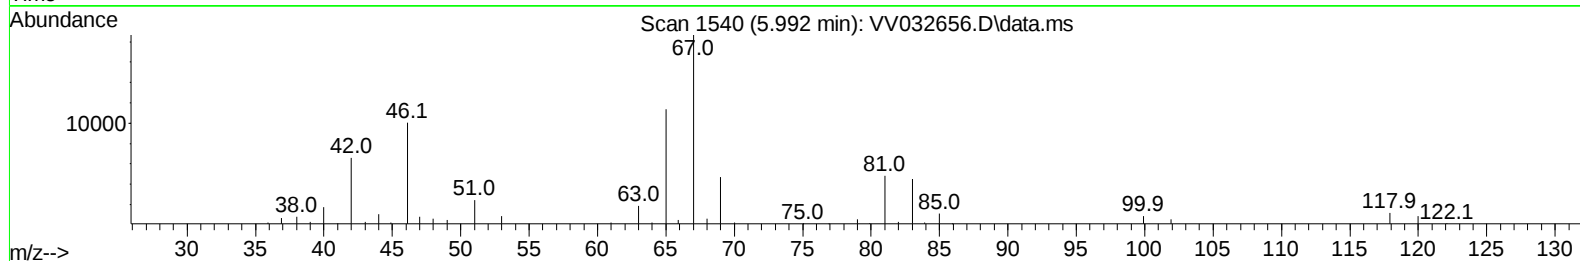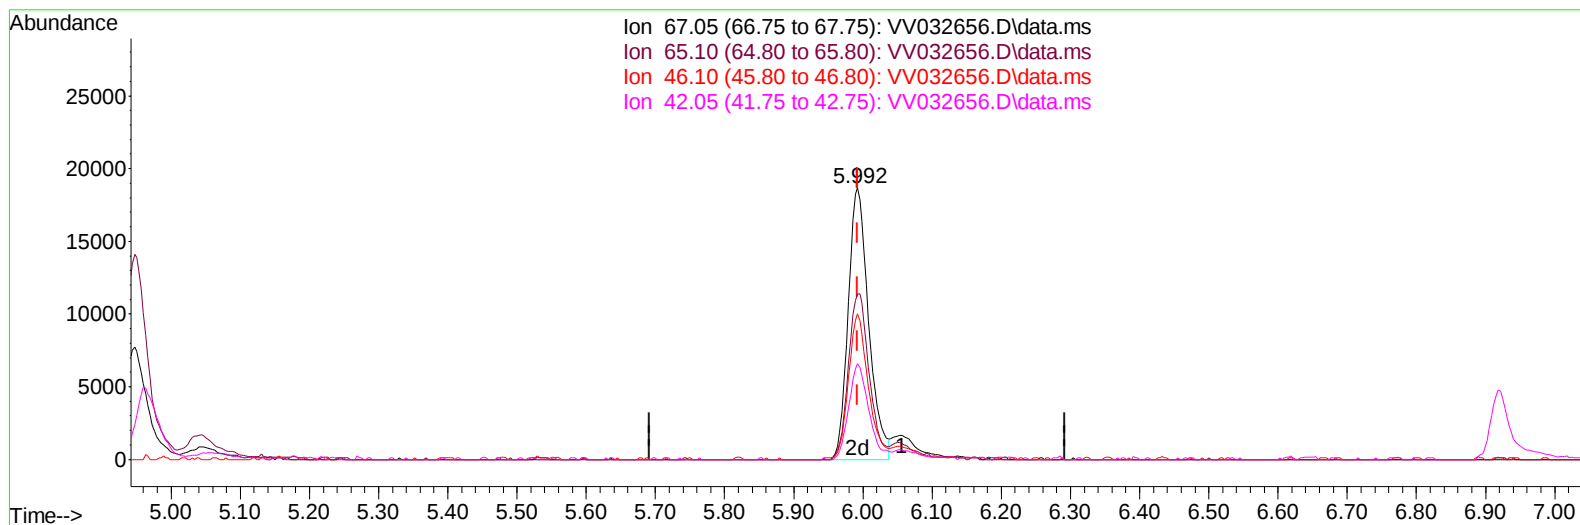

TIC: VV032656.D\data.ms

(36) 1,2-Dichloropropane-d6 (S)

5.992min (+ 0.000) 3.93 ug/L m

response 38514

Ion	Exp%	Act%
67.05	100.00	100.00
65.10	67.60	5.82#
46.10	49.60	3.72#
42.05	26.30	2.96#

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032656.D
 Acq On : 26 Oct 2023 12:41
 Operator : SY/MD
 Sample : 04995-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49K6

Manual IntegrationsAPPROVED

Quant Time: Oct 27 05:34:47 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 27 05:30:38 2023
 Response via : Initial Calibration

Reviewed By :John Carlone 10/27/2023
 Supervised By :Mahesh Dadoda 10/27/2023

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	5.539	114		86901	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.786	117		100437	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152		42375	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.278	65		33081	4.681	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	93.600%	
7) Chloroethane-d5	1.532	69		33262	5.798	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	116.000%	
11) 1,1-Dichloroethene-d2	2.060	65		13168	4.418	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	88.400%	
20) 2-Butanone-d5	3.799	46		74344	41.583	ug/L	-0.03
Spiked Amount 50.000	Range 40	- 130		Recovery	=	83.160%	
24) Chloroform-d	4.256	84		61199	4.909	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	98.200%	
26) 1,2-Dichloroethane-d4	4.947	65		31289	5.298	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	106.000%	
32) Benzene-d6	4.963	84		117153	3.964	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	79.200%	
36) 1,2-Dichloropropane-d6	5.992	67		38514m	3.933	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	78.600%	
41) Toluene-d8	7.246	98		107236	3.968	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	79.400%	
43) trans-1,3-Dichloroprop...	7.561	79		13322	3.839	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	76.800%	
46) 2-Hexanone-d5	8.027	63		62849	38.498	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	77.000%	
56) 1,1,2,2-Tetrachloroeth...	10.156	84		32081	4.684	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	93.600%	
66) 1,2-Dichlorobenzene-d4	11.564	152		41041	5.219	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	104.400%	
Target Compounds							
						Qvalue	
3) Chloromethane	1.217	50		8219	0.842	ug/L	99
13) Acetone	2.127	43		3295	2.391	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032656.D
Acq On : 26 Oct 2023 12:41
Operator : SY/MD
Sample : 04995-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49K6

Manual IntegrationsAPPROVED

Quant Time: Oct 27 05:34:47 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 27 05:30:38 2023
Response via : Initial Calibration

Reviewed By :John Carlone 10/27/2023
Supervised By :Mahesh Dadoda 10/27/2023

