

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102623\
 Data File : VW032665.D
 Acq On : 26 Oct 2023 16:12
 Operator : SY/MD
 Sample : 05009-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4995

Quant Time: Oct 27 05:37:34 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Oct 27 05:30:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	86148	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	98263	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.188	152	42949	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	29224	4.171	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.400%
7) Chloroethane-d5	1.532	69	30234	5.316	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	106.400%
11) 1,1-Dichloroethene-d2	2.060	65	11914	4.032	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	80.600%
20) 2-Butanone-d5	3.799	46	66143	37.319	ug/L	-0.03
Spiked Amount	50.000	Range	40 - 130	Recovery	=	74.640%
24) Chloroform-d	4.252	84	53029	4.290	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	85.800%
26) 1,2-Dichloroethane-d4	4.950	65	28577	4.881	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.600%
32) Benzene-d6	4.963	84	105414	3.646	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	73.000%
36) 1,2-Dichloropropane-d6	5.992	67	34428	3.594	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	71.800%
41) Toluene-d8	7.246	98	94281	3.566	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	71.400%
43) trans-1,3-Dichloroprop...	7.561	79	11221	3.305	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	66.200%
46) 2-Hexanone-d5	8.030	63	54085	33.862	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	67.720%
56) 1,1,2,2-Tetrachloroeth...	10.156	84	28611	4.270	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	85.400%
66) 1,2-Dichlorobenzene-d4	11.564	152	36577	4.589	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	91.800%
Target Compounds						
13) Acetone	2.127	43	3277	2.399	ug/L	Qvalue 89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032665.D
Acq On : 26 Oct 2023 16:12
Operator : SY/MD
Sample : 05009-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4995

Quant Time: Oct 27 05:37:34 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Oct 27 05:30:38 2023
Response via : Initial Calibration

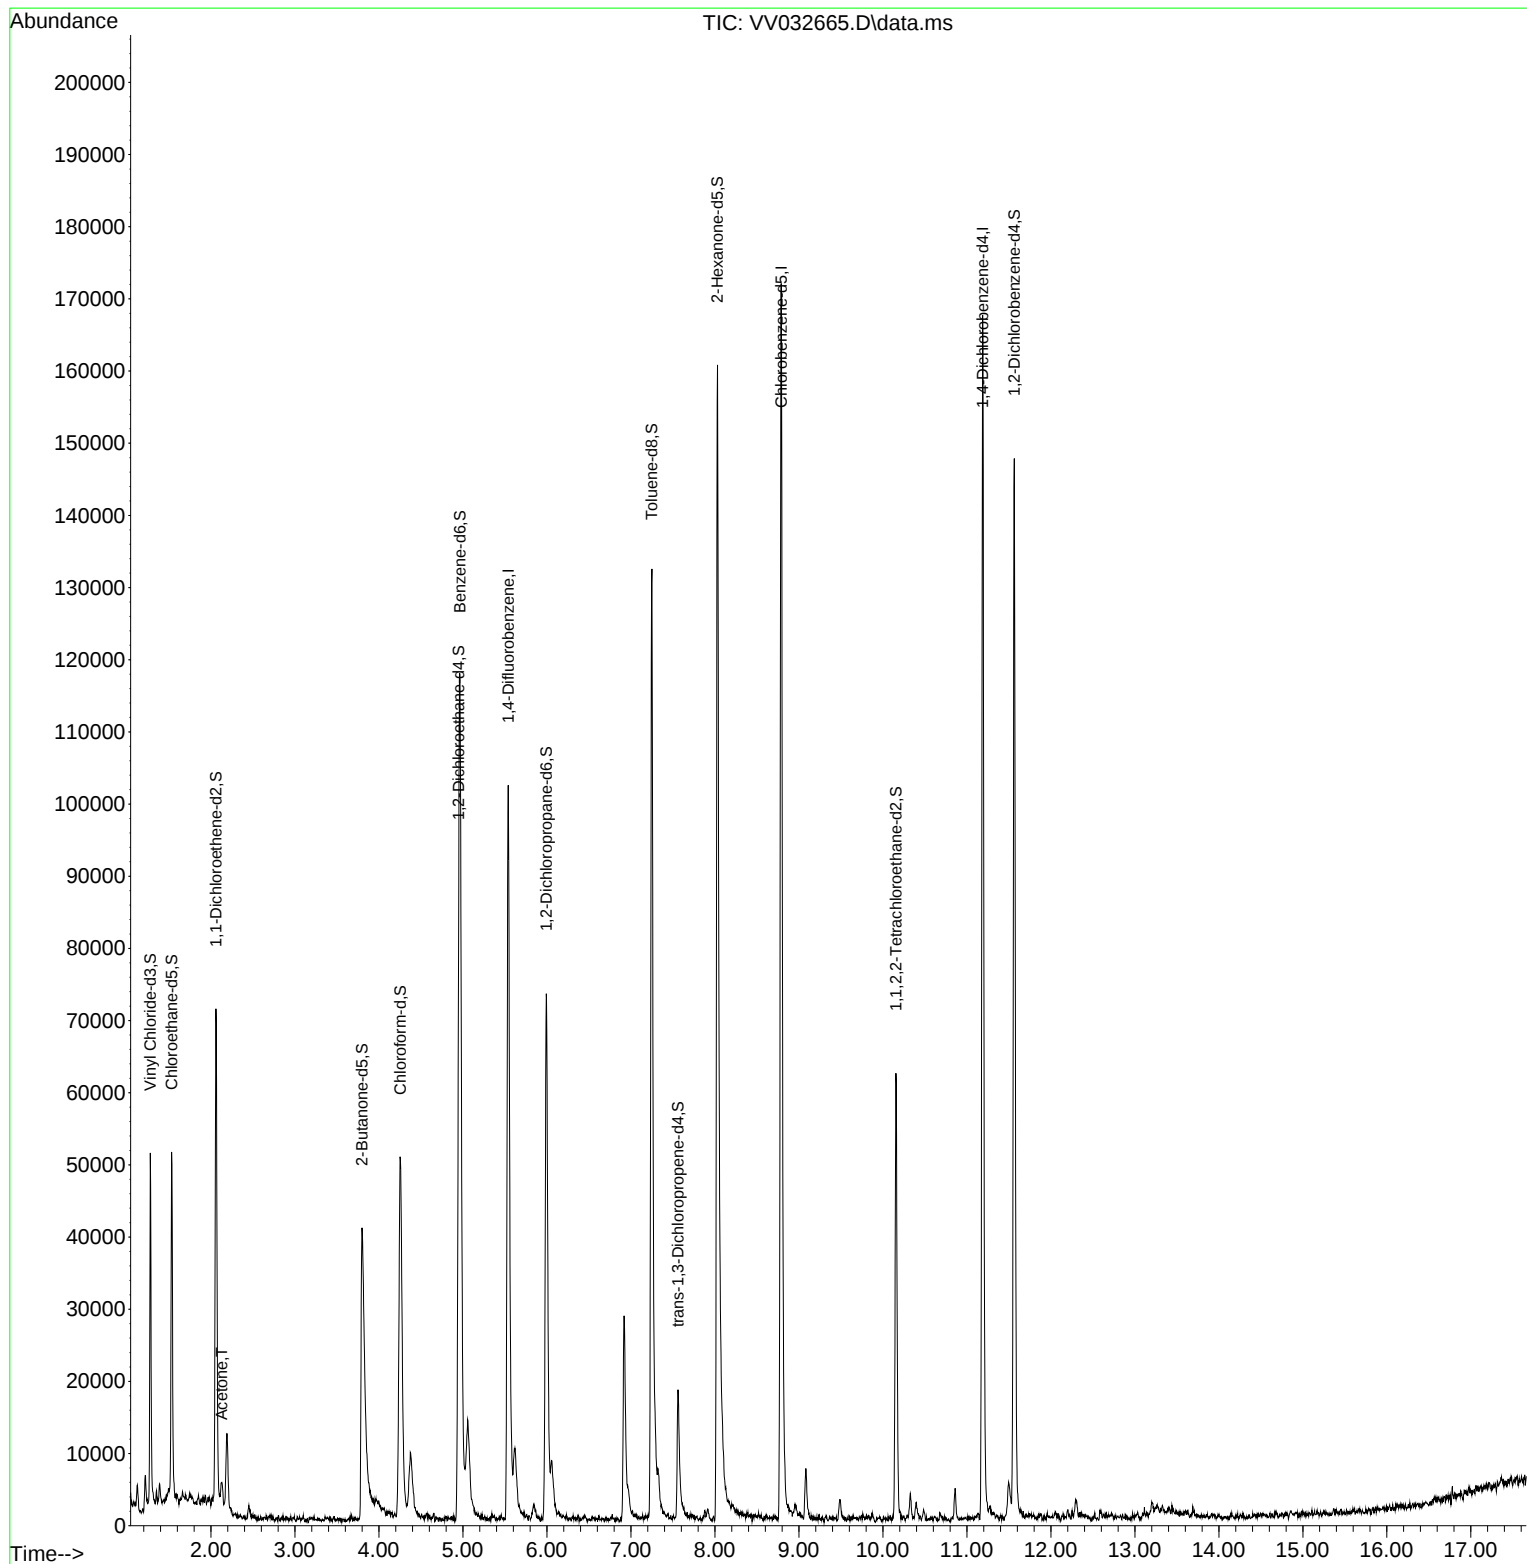

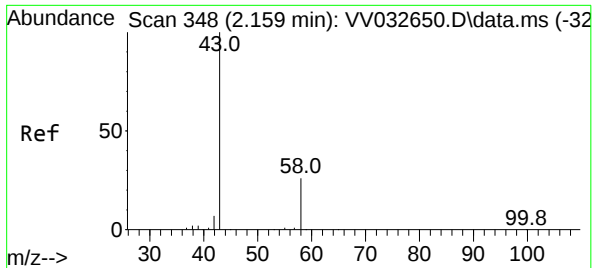

#13
 Acetone
 Concen: 2.399 ug/L
 RT: 2.127 min Scan# 31
 Delta R.T. -0.032 min
 Lab File: VV032665.D
 Acq: 26 Oct 2023 16:12

Instrument :
 MSVOA_V
 ClientSampleId :
 A4995

Tgt Ion: 43 Resp: 3277
 Ion Ratio Lower Upper
 43 100
 58 26.8 0.0 66.0

