

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032651.D
 Acq On : 26 Oct 2023 10:41
 Operator : SY/MD
 Sample : VV1026WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK381

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	19	27	35	rVB	4302	5741	1.47%	0.191%
2	1.275	66	73	86	rVV	53118	58012	14.83%	1.931%
3	1.532	145	153	165	rBV	48755	57976	14.82%	1.929%
4	2.056	306	316	327	rBV	80182	114535	29.28%	3.811%
5	2.188	348	357	369	rBV2	12323	22709	5.81%	0.756%
6	3.831	855	868	870	rBV2	24272	41812	10.69%	1.391%
7	4.252	983	999	1024	rBV	52475	137557	35.17%	4.578%
8	4.378	1024	1038	1055	rVB3	10446	28453	7.27%	0.947%
9	4.960	1204	1219	1238	rBV2	130243	326782	83.55%	10.875%
10	5.056	1240	1249	1273	rVB7	14172	43255	11.06%	1.439%
11	5.535	1388	1398	1415	rBV	108946	230315	58.88%	7.664%
12	5.616	1420	1423	1440	rVB2	10199	19827	5.07%	0.660%
13	5.992	1528	1540	1555	rBV2	77333	165856	42.40%	5.519%
14	6.918	1818	1828	1844	rBV	34049	68975	17.63%	2.295%
15	7.246	1916	1930	1955	rBV	144965	284485	72.73%	9.467%
16	7.561	2017	2028	2053	rBV3	21594	48081	12.29%	1.600%
17	8.034	2165	2175	2210	rBV	170012	391137	100.00%	13.016%
18	8.789	2399	2410	2436	rBV	184805	326451	83.46%	10.864%
19	10.156	2821	2835	2854	rBV	66445	113204	28.94%	3.767%
20	11.188	3145	3156	3174	rBV	174407	275506	70.44%	9.168%
21	11.564	3262	3273	3290	rBV	148503	244325	62.47%	8.131%




Sum of corrected areas: 3004994

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032651.D
Acq On : 26 Oct 2023 10:41
Operator : SY/MD
Sample : VV1026WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

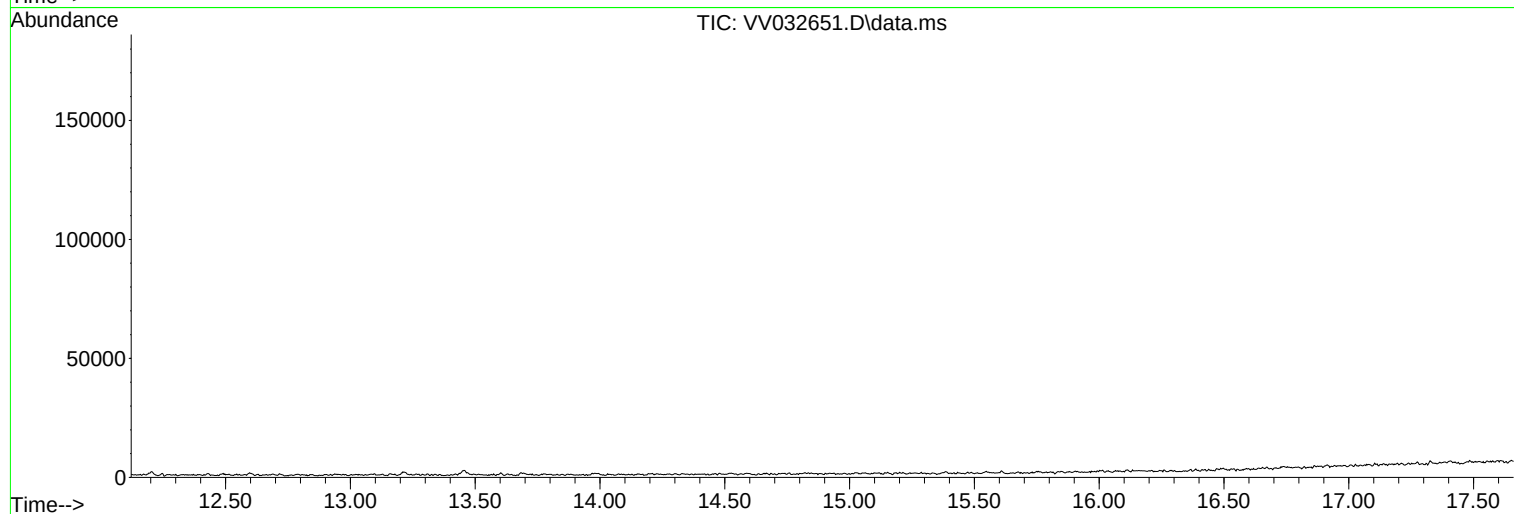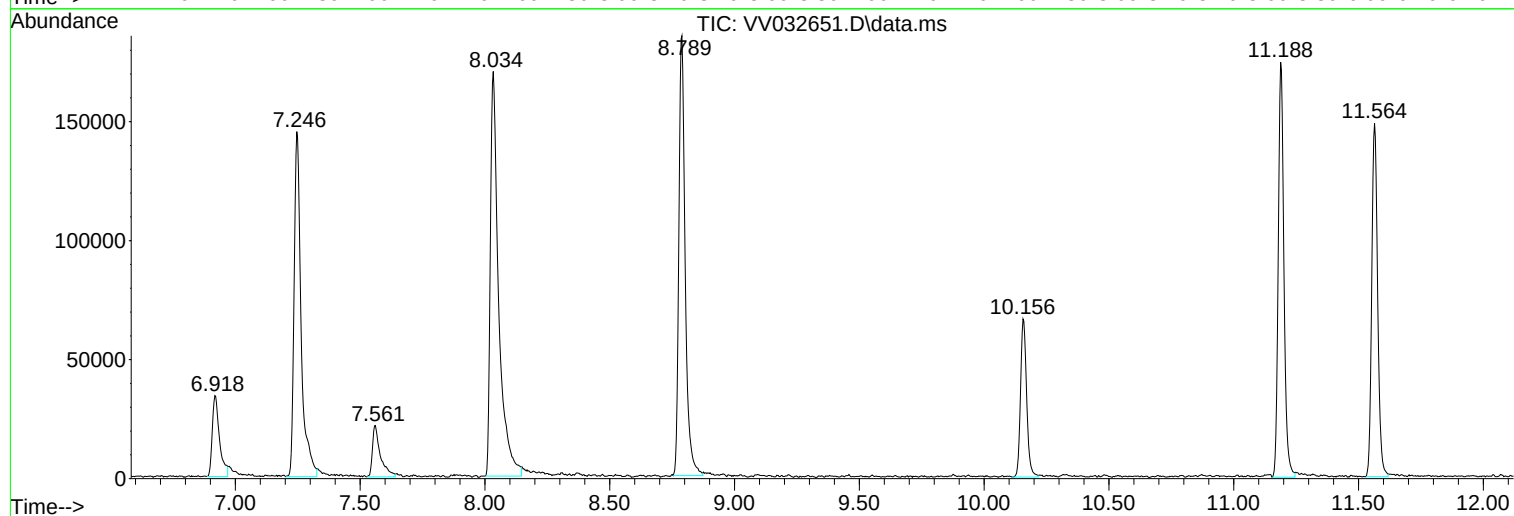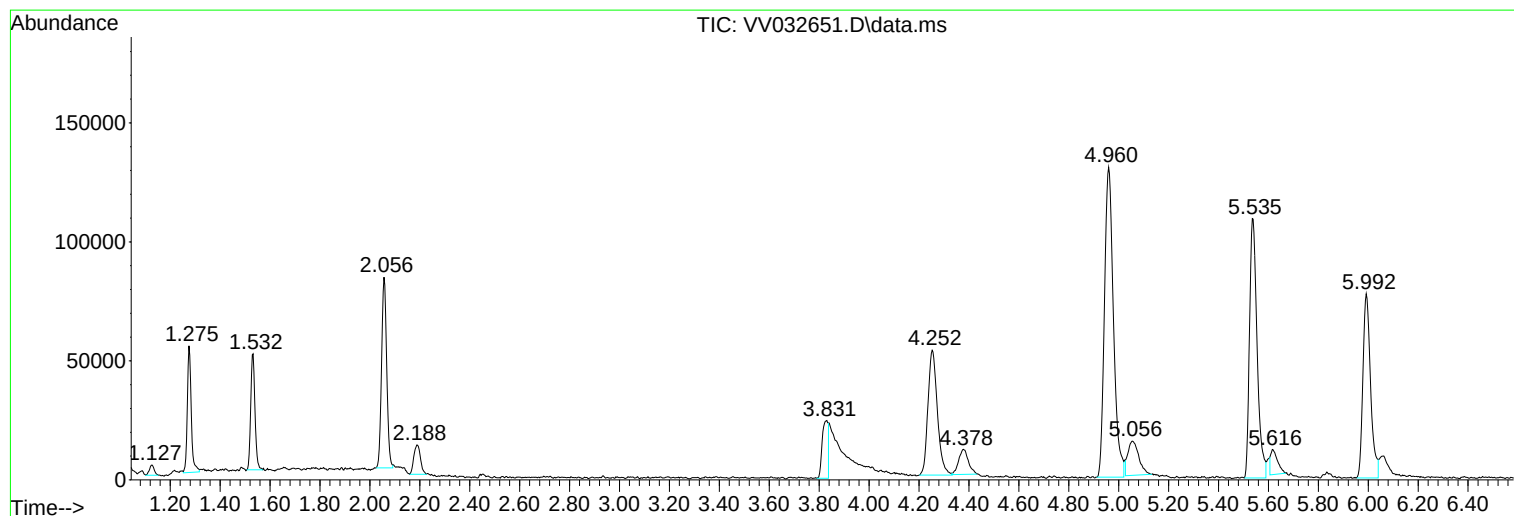

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032651.D
Acq On : 26 Oct 2023 10:41
Operator : SY/MD
Sample : VV1026WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032651.D
Acq On : 26 Oct 2023 10:41
Operator : SY/MD
Sample : VV1026WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK381

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc