

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032652.D
 Acq On : 26 Oct 2023 11:06
 Operator : SY/MD
 Sample : 04962-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032652.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	20	27	39	rVB	4385	6697	1.77%	0.221%
2	1.278	66	74	85	rBV	50626	52672	13.91%	1.739%
3	1.532	145	153	169	rVB	48595	58765	15.52%	1.940%
4	2.059	308	317	335	rVB	75167	112142	29.61%	3.702%
5	2.195	348	359	370	rBV	12349	22140	5.85%	0.731%
6	3.812	852	862	893	rBV	25853	97162	25.65%	3.207%
7	4.252	985	999	1020	rBV2	51309	135646	35.81%	4.477%
8	4.381	1024	1039	1056	rVB4	10973	29184	7.71%	0.963%
9	4.960	1204	1219	1239	rBV3	125716	322982	85.27%	10.661%
10	5.059	1240	1250	1279	rVB6	14320	45063	11.90%	1.487%
11	5.538	1384	1399	1418	rBV	106705	228929	60.44%	7.556%
12	5.619	1418	1424	1438	rVB3	9137	21071	5.56%	0.696%
13	5.992	1524	1540	1554	rBV2	76304	161939	42.76%	5.345%
14	6.918	1815	1828	1842	rBV	34053	67354	17.78%	2.223%
15	7.246	1918	1930	1961	rBV	139224	279403	73.77%	9.222%
16	7.561	2019	2028	2057	rBV2	20645	45278	11.95%	1.495%
17	8.030	2163	2174	2204	rBV	153210	378758	100.00%	12.502%
18	8.789	2398	2410	2439	rBV	181158	323590	85.43%	10.681%
19	10.156	2821	2835	2853	rBV	65037	110868	29.27%	3.660%
20	11.188	3146	3156	3181	rBV	173786	279516	73.80%	9.226%
21	11.564	3258	3273	3294	rBV	153082	250422	66.12%	8.266%




Sum of corrected areas: 3029581

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032652.D
Acq On : 26 Oct 2023 11:06
Operator : SY/MD
Sample : 04962-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

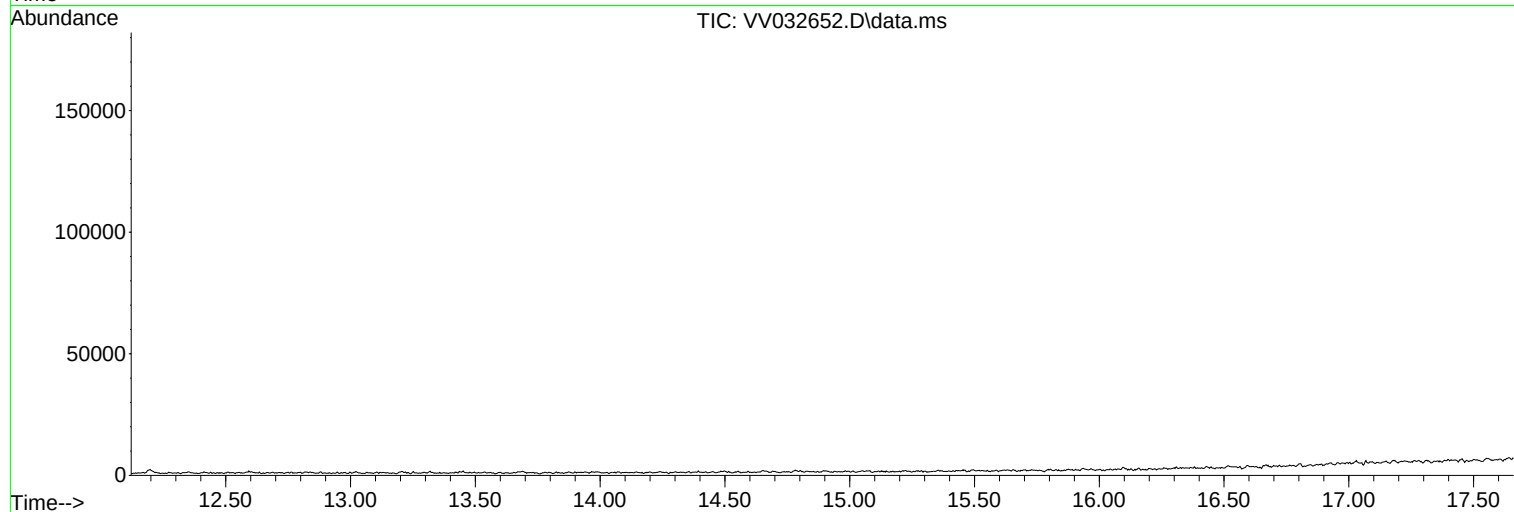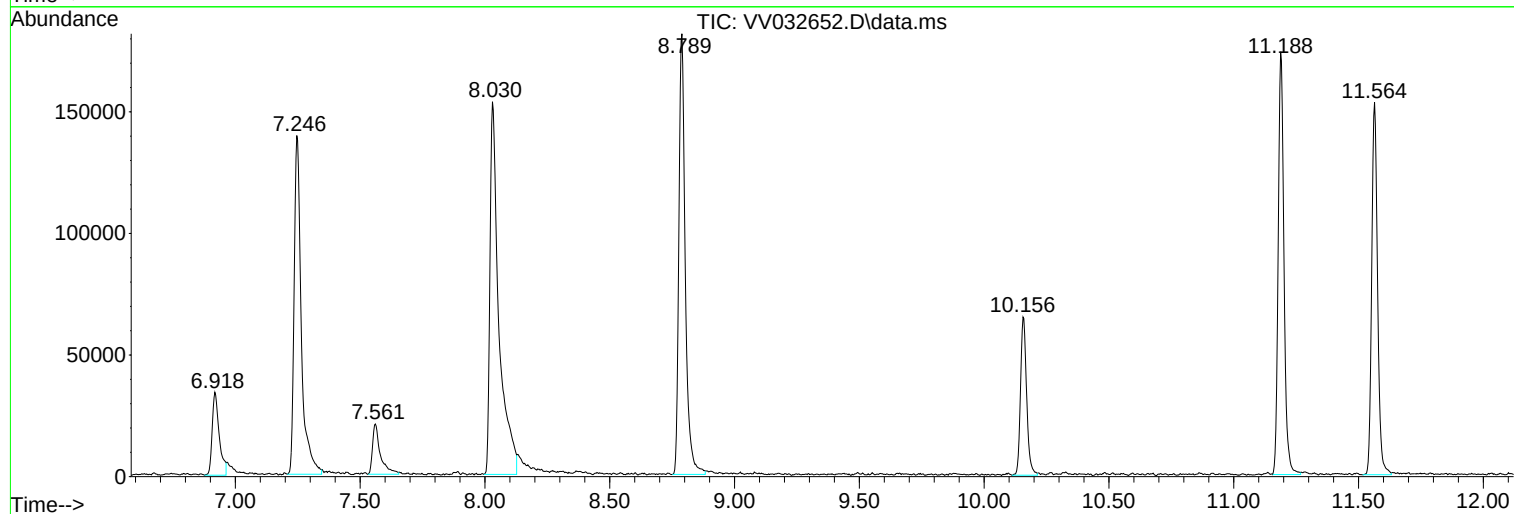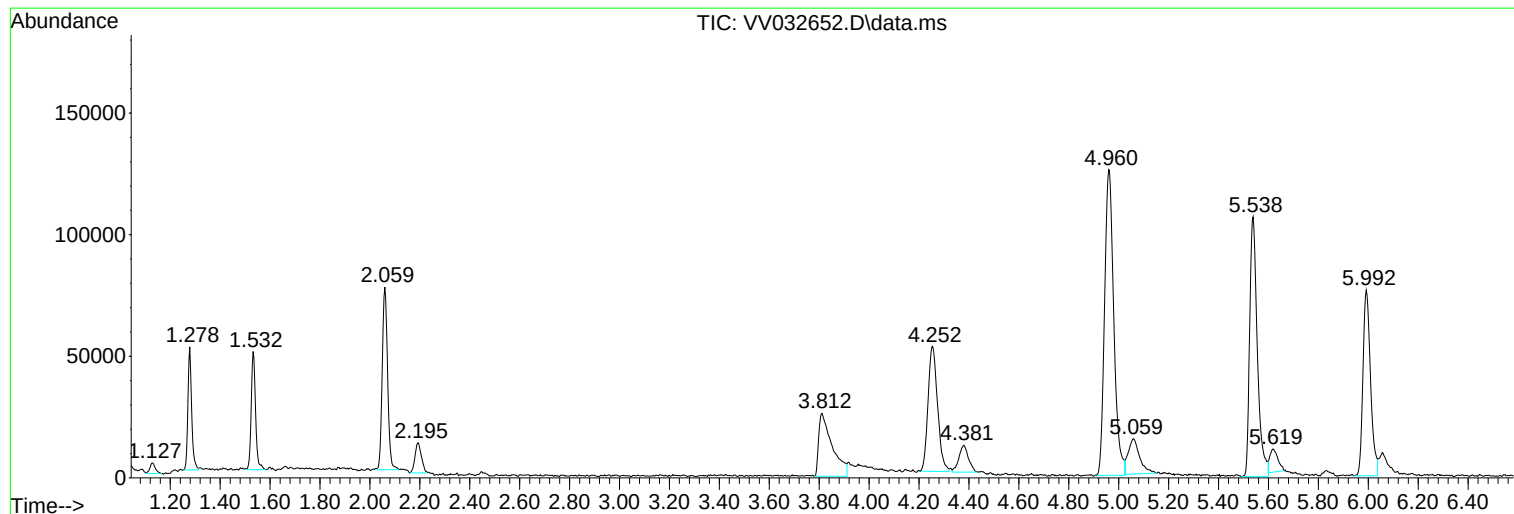

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032652.D
Acq On : 26 Oct 2023 11:06
Operator : SY/MD
Sample : 04962-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032652.D
Acq On : 26 Oct 2023 11:06
Operator : SY/MD
Sample : 04962-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc