

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032653.D
 Acq On : 26 Oct 2023 11:30
 Operator : SY/MD
 Sample : 04961-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032653.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	19	25	34	rVB	4922	6340	1.68%	0.212%
2	1.278	67	74	89	rBV	48484	53356	14.12%	1.785%
3	1.532	146	153	165	rBV	47947	56337	14.91%	1.884%
4	2.060	306	317	330	rBV	74084	107995	28.59%	3.612%
5	2.188	348	357	368	rVB	12585	21553	5.71%	0.721%
6	3.809	852	861	887	rBV2	25499	88717	23.49%	2.967%
7	4.253	982	999	1022	rBV	53959	140933	37.31%	4.714%
8	4.375	1026	1037	1052	rVB2	9792	24581	6.51%	0.822%
9	4.960	1204	1219	1238	rBV2	129374	328380	86.93%	10.984%
10	5.056	1242	1249	1272	rVB5	13616	36575	9.68%	1.223%
11	5.539	1386	1399	1416	rBV	103276	217646	57.62%	7.280%
12	5.616	1416	1423	1437	rVB2	8491	19903	5.27%	0.666%
13	5.992	1525	1540	1555	rBV	78444	168148	44.51%	5.624%
14	6.918	1818	1828	1854	rBV	35026	75212	19.91%	2.516%
15	7.246	1919	1930	1955	rBV	141175	281288	74.46%	9.409%
16	7.561	2016	2028	2050	rBV2	20822	44936	11.90%	1.503%
17	8.030	2164	2174	2208	rBV	147968	377748	100.00%	12.635%
18	8.789	2396	2410	2437	rBV	172324	313466	82.98%	10.485%
19	10.156	2823	2835	2851	rBV	66077	109529	29.00%	3.664%
20	11.188	3145	3156	3177	rBV	167182	268574	71.10%	8.983%
21	11.564	3260	3273	3288	rBV	153628	248464	65.78%	8.311%




Sum of corrected areas: 2989681

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032653.D
Acq On : 26 Oct 2023 11:30
Operator : SY/MD
Sample : 04961-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

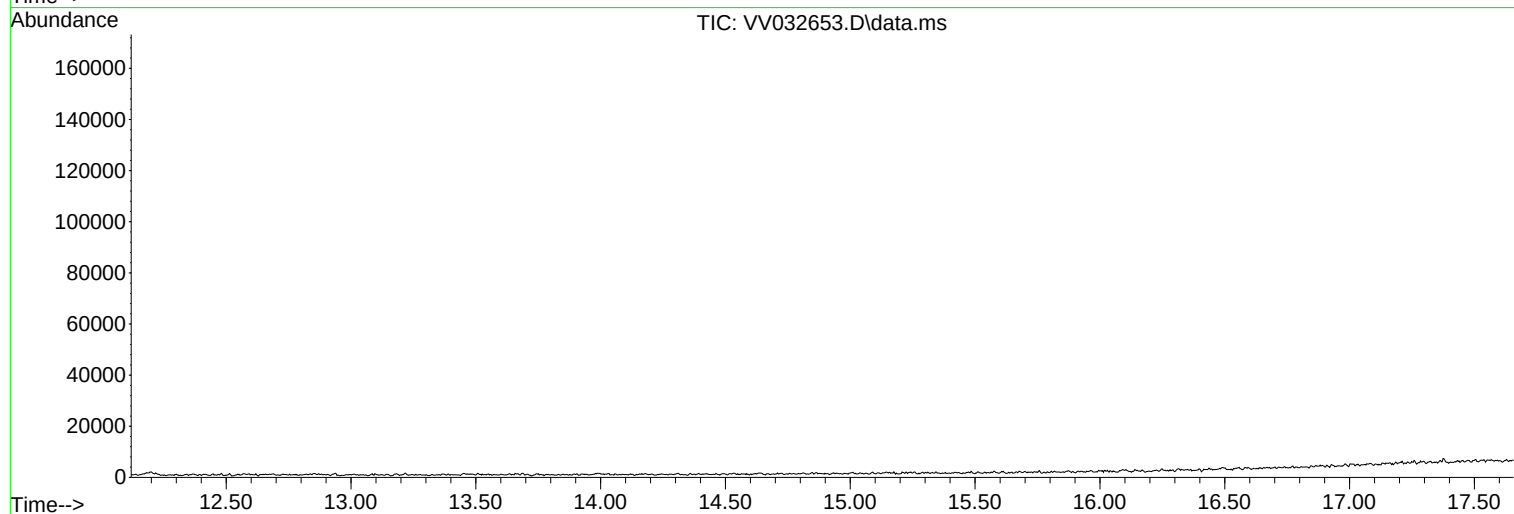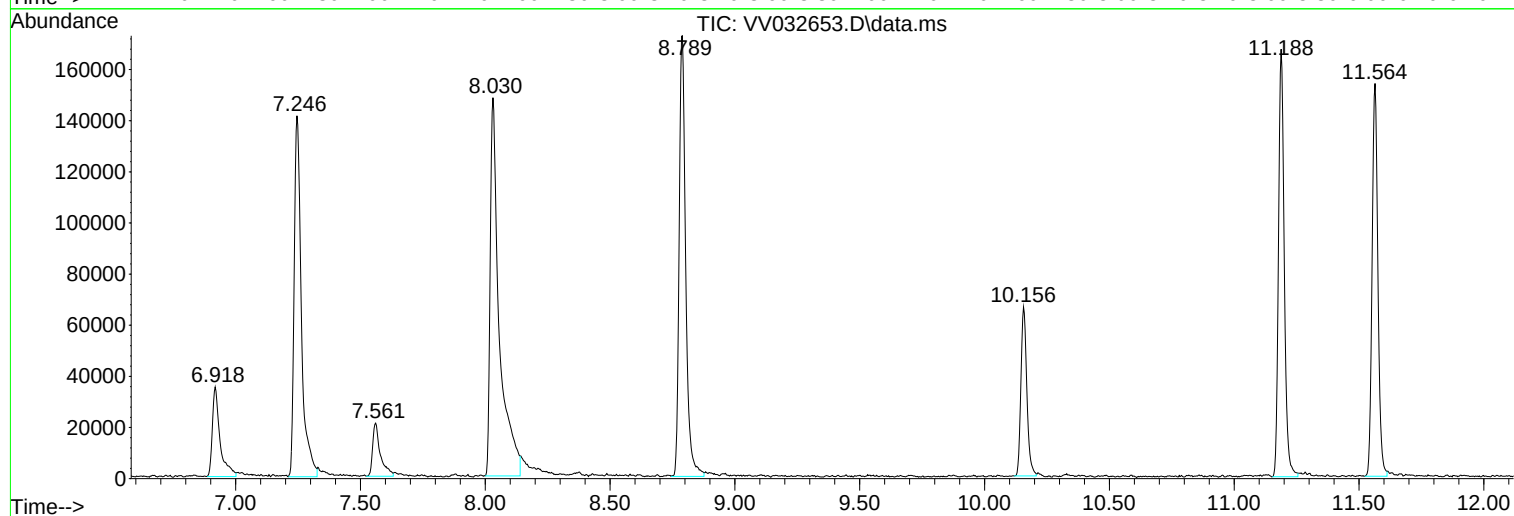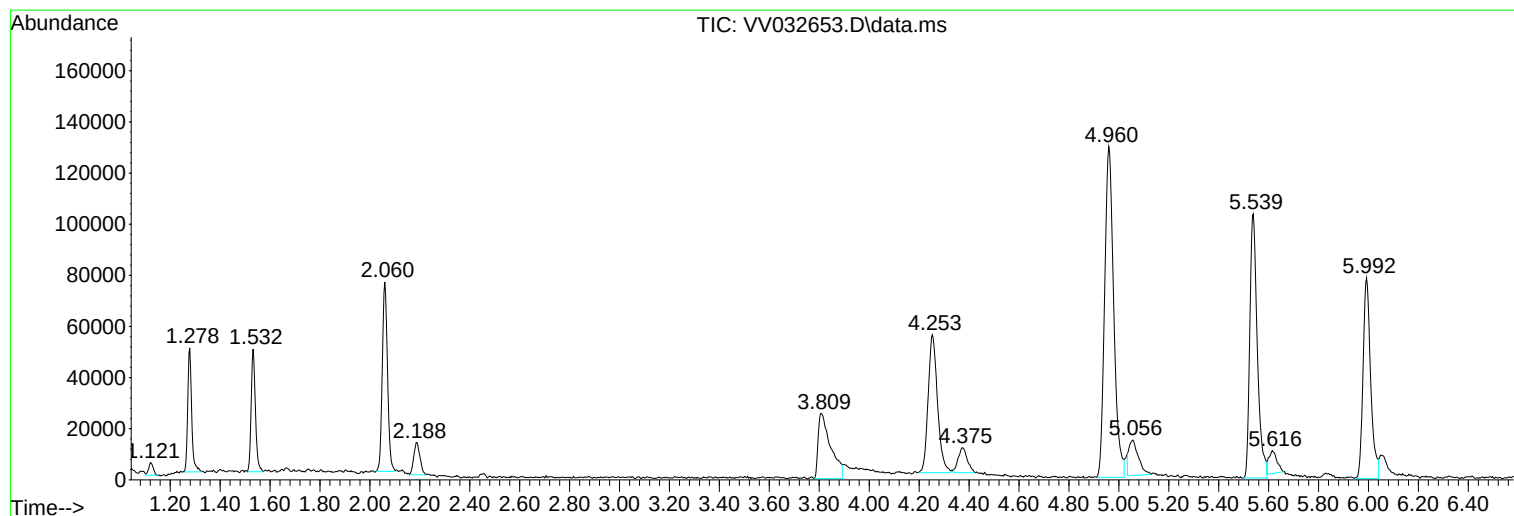

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032653.D
Acq On : 26 Oct 2023 11:30
Operator : SY/MD
Sample : 04961-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032653.D
Acq On : 26 Oct 2023 11:30
Operator : SY/MD
Sample : 04961-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
