

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032654.D
 Acq On : 26 Oct 2023 11:54
 Operator : SY/MD
 Sample : 04995-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49C8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032654.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	32	rVB	3547	4288	1.17%	0.143%
2	1.217	49	55	65	rBV	7117	9020	2.46%	0.301%
3	1.278	65	74	88	rVV	49167	54154	14.77%	1.805%
4	1.388	102	108	114	rVB	4020	4293	1.17%	0.143%
5	1.532	144	153	163	rBV	48781	57551	15.70%	1.918%
6	2.060	307	317	329	rBV	73326	108600	29.62%	3.620%
7	2.185	347	356	369	rVB3	10332	20450	5.58%	0.682%
8	3.806	846	860	884	rBV2	47736	159117	43.40%	5.303%
9	4.253	982	999	1024	rBV2	52914	142600	38.89%	4.753%
10	4.368	1024	1035	1058	rVB2	8310	24264	6.62%	0.809%
11	4.960	1204	1219	1240	rBV2	123177	319091	87.03%	10.635%
12	5.053	1241	1248	1266	rVB5	10953	28584	7.80%	0.953%
13	5.535	1387	1398	1416	rBV	102861	219897	59.97%	7.329%
14	5.616	1418	1423	1443	rVB4	8837	22090	6.02%	0.736%
15	5.992	1526	1540	1553	rBV	74337	155680	42.46%	5.189%
16	6.050	1555	1558	1569	rVB6	6349	10434	2.85%	0.348%
17	6.918	1817	1828	1849	rBV	29704	64427	17.57%	2.147%
18	7.246	1918	1930	1953	rBV	137033	265751	72.48%	8.857%
19	7.561	2017	2028	2042	rBV3	18911	39118	10.67%	1.304%
20	8.031	2163	2174	2213	rBV	167858	366651	100.00%	12.220%
21	8.786	2395	2409	2437	rBV	174886	310749	84.75%	10.357%
22	9.082	2495	2501	2514	rVB9	3770	6612	1.80%	0.220%
23	10.156	2825	2835	2852	rBV	63583	102309	27.90%	3.410%
24	10.860	3046	3054	3060	rBV8	2432	3775	1.03%	0.126%
25	11.188	3144	3156	3177	rBV	167618	266121	72.58%	8.870%
26	11.564	3262	3273	3291	rBV	144358	234681	64.01%	7.822%




Sum of corrected areas: 3000307

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032654.D
Acq On : 26 Oct 2023 11:54
Operator : SY/MD
Sample : 04995-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49C8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

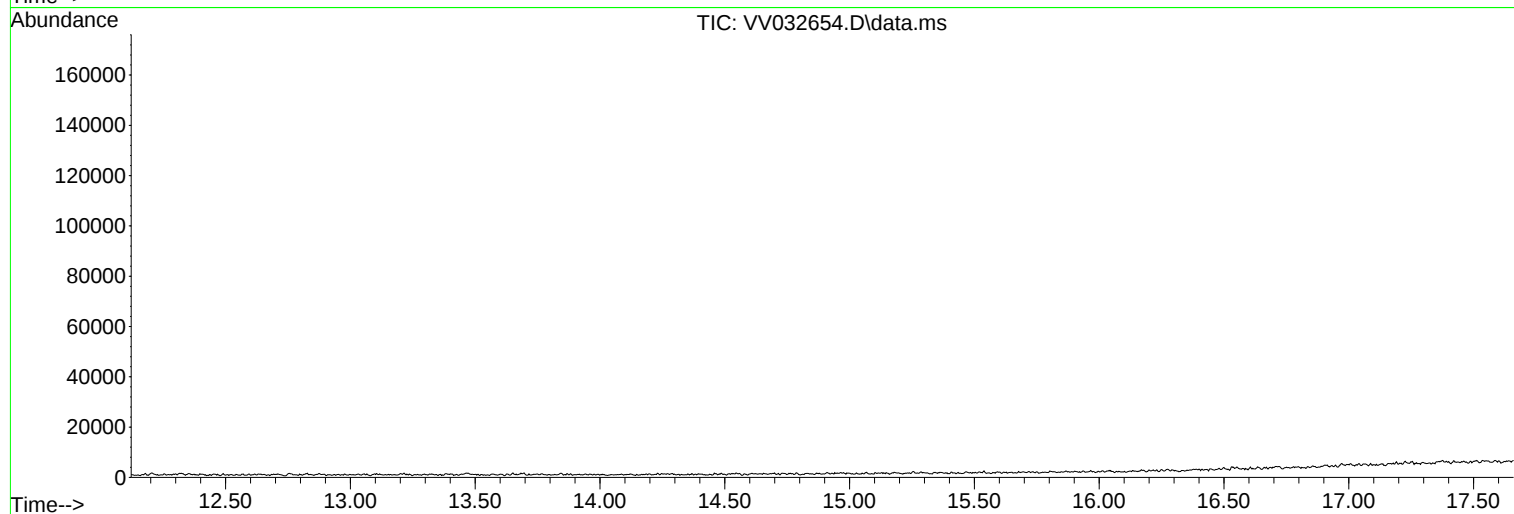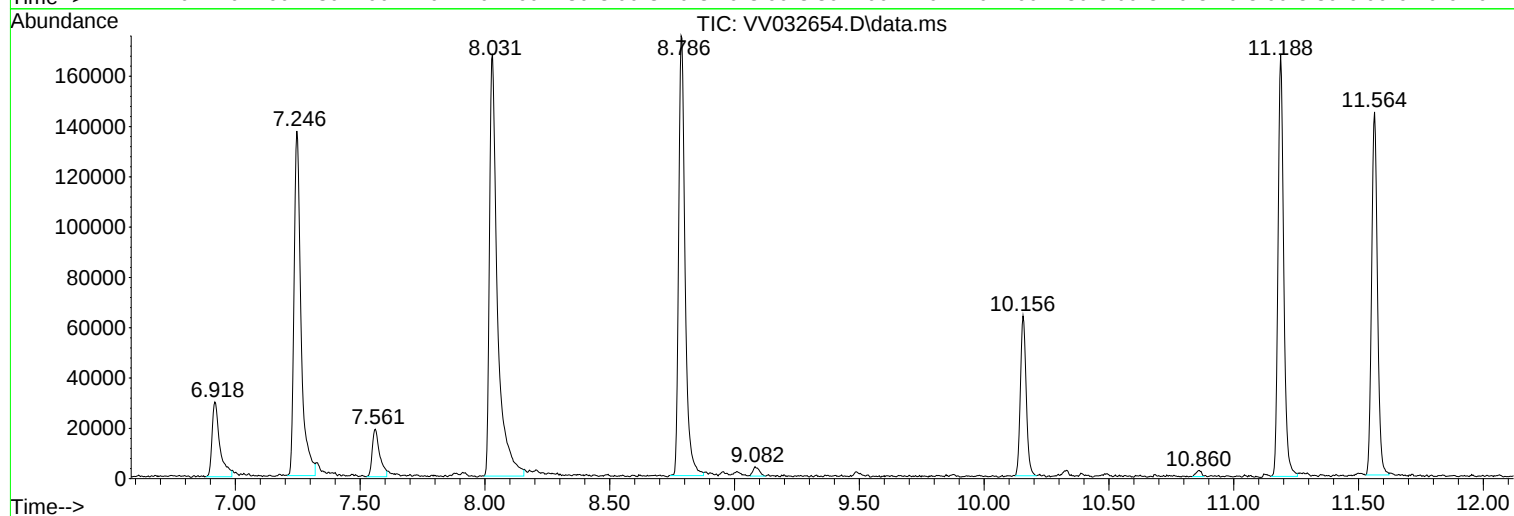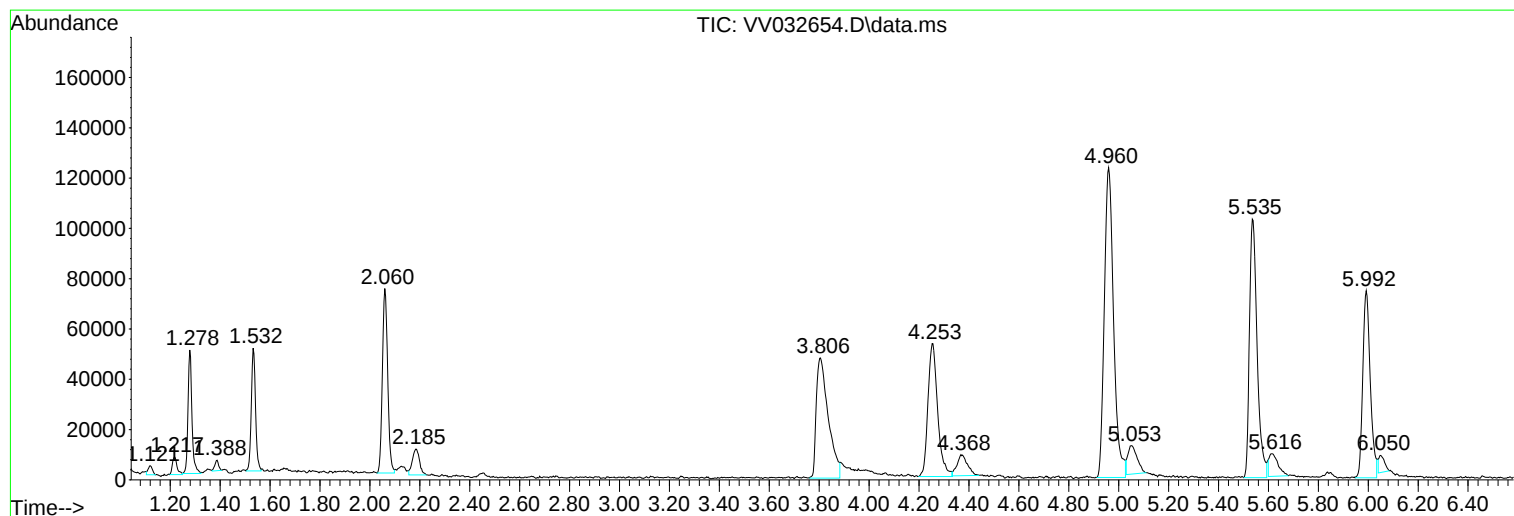

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032654.D
Acq On : 26 Oct 2023 11:54
Operator : SY/MD
Sample : 04995-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49C8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032654.D
Acq On : 26 Oct 2023 11:54
Operator : SY/MD
Sample : 04995-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49C8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
