

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032656.D
 Acq On : 26 Oct 2023 12:41
 Operator : SY/MD
 Sample : 04995-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49K6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032656.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	34	rVB	3361	5076	1.29%	0.159%
2	1.217	47	55	62	rBV	12731	15854	4.04%	0.496%
3	1.278	67	74	89	rVB	52125	57278	14.61%	1.794%
4	1.384	102	107	114	rBV	4932	5891	1.50%	0.184%
5	1.420	114	118	127	rVB7	3638	4234	1.08%	0.133%
6	1.536	145	154	167	rVB	53847	65673	16.75%	2.057%
7	2.060	307	317	331	rBV	78842	117316	29.92%	3.674%
8	2.127	332	338	345	rVV3	3569	6608	1.69%	0.207%
9	2.185	347	356	368	rVB	10978	21507	5.49%	0.674%
10	3.802	847	859	887	rBV2	52146	173923	44.36%	5.447%
11	4.253	983	999	1020	rBV	57643	152625	38.93%	4.780%
12	4.372	1027	1036	1054	rVB3	7790	21477	5.48%	0.673%
13	4.960	1204	1219	1238	rBV3	131287	337580	86.10%	10.572%
14	5.050	1240	1247	1267	rVB4	11927	33758	8.61%	1.057%
15	5.539	1385	1399	1416	rBV	102746	215831	55.05%	6.759%
16	5.613	1417	1422	1438	rVB4	8305	19775	5.04%	0.619%
17	5.992	1528	1540	1553	rBV2	80144	167343	42.68%	5.241%
18	6.918	1816	1828	1843	rBV	33611	67393	17.19%	2.110%
19	7.246	1920	1930	1965	rBV	150209	294128	75.02%	9.211%
20	7.558	2019	2027	2046	rBV2	20277	41113	10.49%	1.287%
21	8.031	2162	2174	2210	rBV	181648	392072	100.00%	12.278%
22	8.786	2397	2409	2431	rBV	174396	307370	78.40%	9.626%
23	9.008	2472	2478	2489	rBV7	2795	4012	1.02%	0.126%
24	10.156	2824	2835	2850	rBV2	68396	111883	28.54%	3.504%
25	11.188	3145	3156	3174	rBV	166349	265419	67.70%	8.312%
26	11.490	3238	3250	3262	rBV5	8625	20909	5.33%	0.655%
27	11.564	3262	3273	3296	rVB	160788	267213	68.15%	8.368%




Sum of corrected areas: 3193261

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032656.D
Acq On : 26 Oct 2023 12:41
Operator : SY/MD
Sample : 04995-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

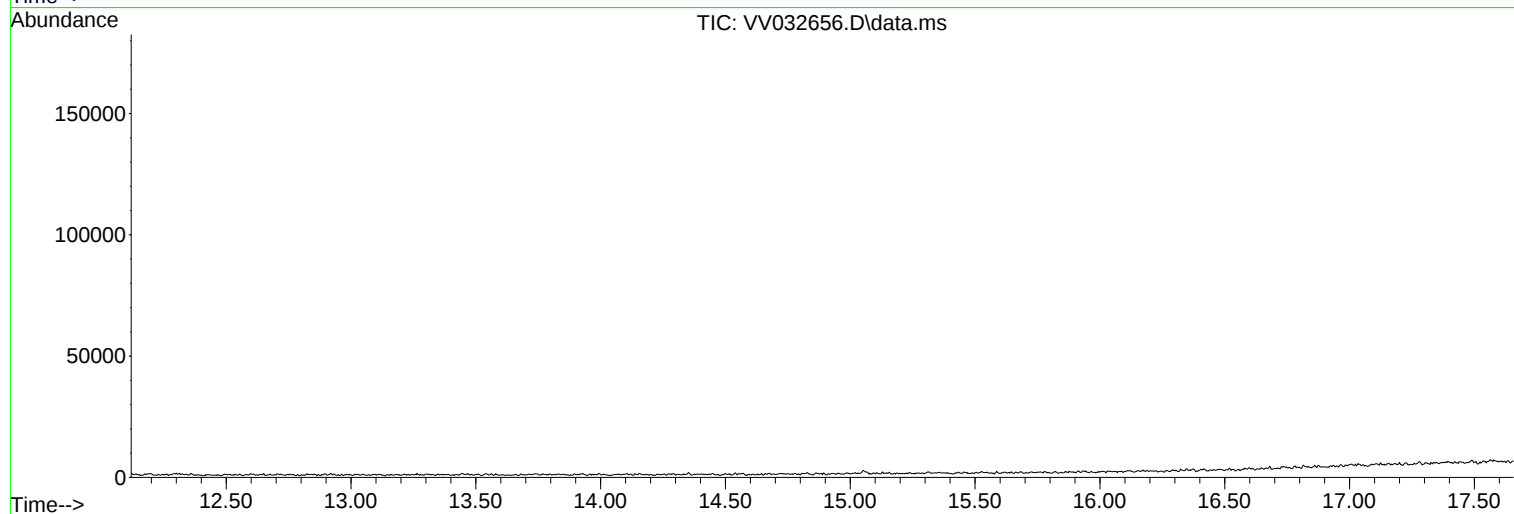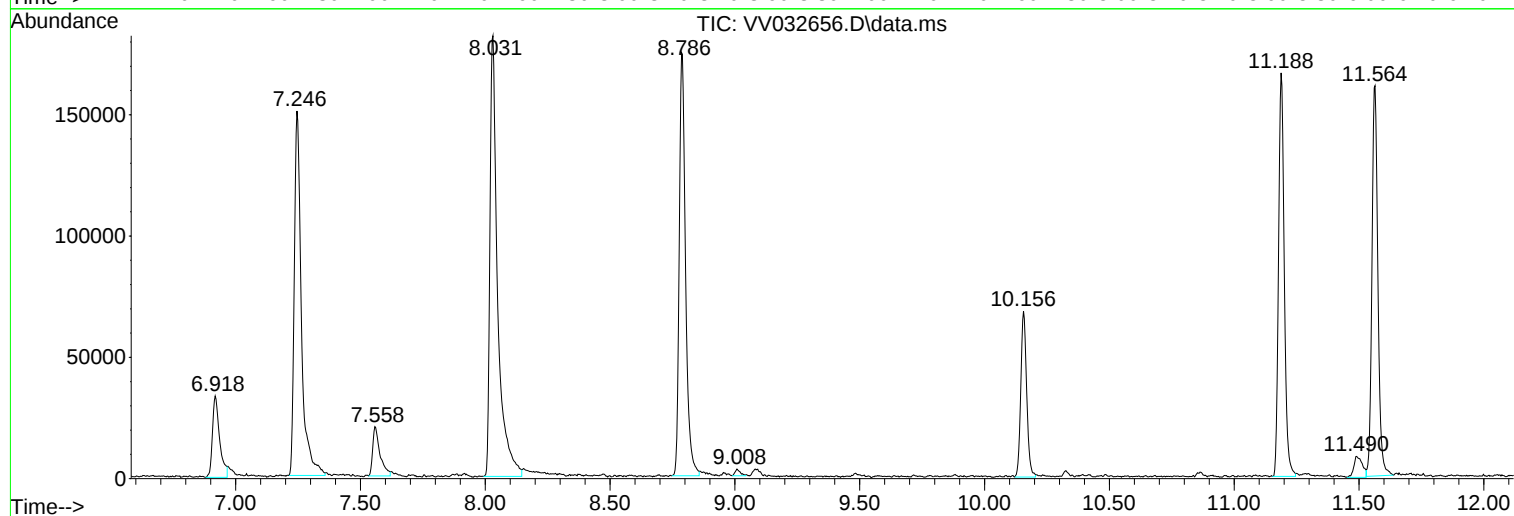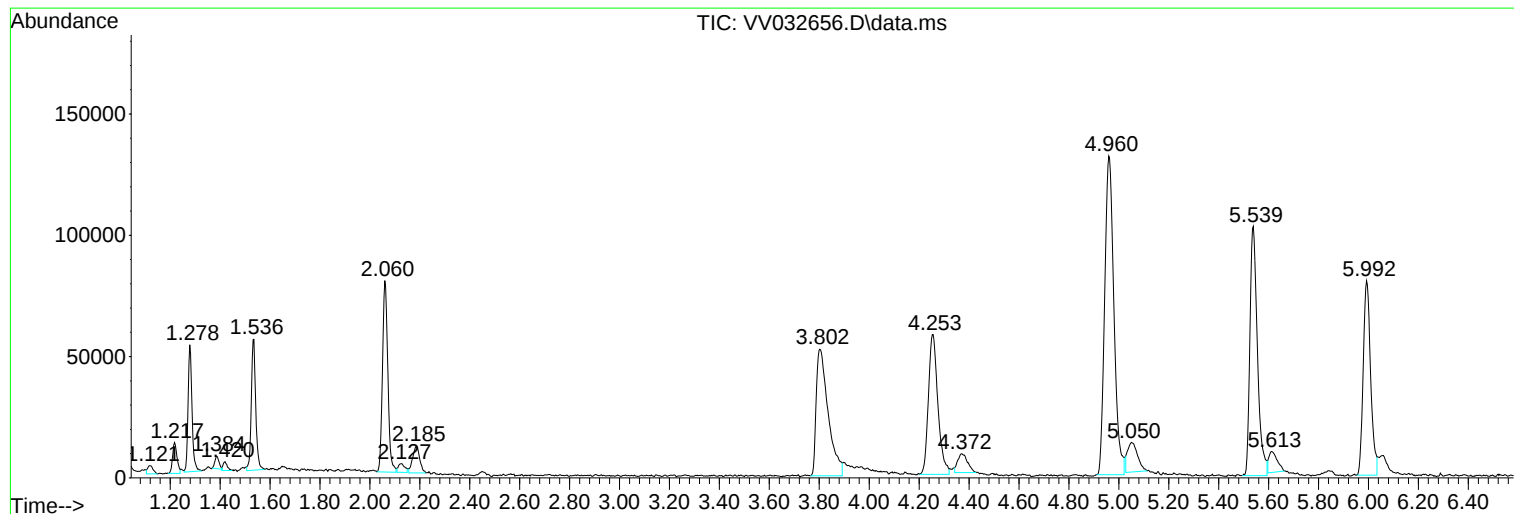

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032656.D
Acq On : 26 Oct 2023 12:41
Operator : SY/MD
Sample : 04995-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032656.D
Acq On : 26 Oct 2023 12:41
Operator : SY/MD
Sample : 04995-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49K6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------