

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032657.D
 Acq On : 26 Oct 2023 13:04
 Operator : SY/MD
 Sample : 04995-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A49L3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032657.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	33	rVB	3415	4489	1.18%	0.147%
2	1.278	67	74	86	rBV	50538	53848	14.12%	1.759%
3	1.532	146	153	168	rBV	49938	61814	16.20%	2.019%
4	2.060	306	317	330	rBV	78071	116150	30.45%	3.794%
5	2.185	347	356	367	rVB	11631	20492	5.37%	0.669%
6	3.799	849	858	891	rBV2	40400	132903	34.84%	4.342%
7	4.256	982	1000	1021	rBV2	55451	148418	38.91%	4.849%
8	4.375	1023	1037	1052	rVB5	7951	22334	5.85%	0.730%
9	4.960	1200	1219	1238	rBV2	131471	335810	88.03%	10.970%
10	5.056	1242	1249	1270	rVB5	13107	35048	9.19%	1.145%
11	5.539	1386	1399	1417	rBV	103095	218726	57.34%	7.145%
12	5.619	1418	1424	1439	rVB4	8292	18360	4.81%	0.600%
13	5.992	1527	1540	1555	rBV2	77899	166248	43.58%	5.431%
14	6.918	1816	1828	1844	rBV	32592	67019	17.57%	2.189%
15	7.246	1920	1930	1949	rBV	148076	283132	74.22%	9.250%
16	7.558	2018	2027	2047	rBV2	19669	41104	10.78%	1.343%
17	8.030	2163	2174	2211	rBV	175235	381471	100.00%	12.462%
18	8.786	2397	2409	2440	rBV	173693	310224	81.32%	10.135%
19	9.079	2494	2500	2502	rBV3	4532	4842	1.27%	0.158%
20	10.156	2823	2835	2850	rBV	67238	108683	28.49%	3.551%
21	11.188	3145	3156	3178	rBV	172214	269944	70.76%	8.819%
22	11.500	3245	3253	3257	rBV7	3401	4792	1.26%	0.157%
23	11.564	3261	3273	3290	rVB	157749	255184	66.89%	8.337%




Sum of corrected areas: 3061035

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032657.D
Acq On : 26 Oct 2023 13:04
Operator : SY/MD
Sample : 04995-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

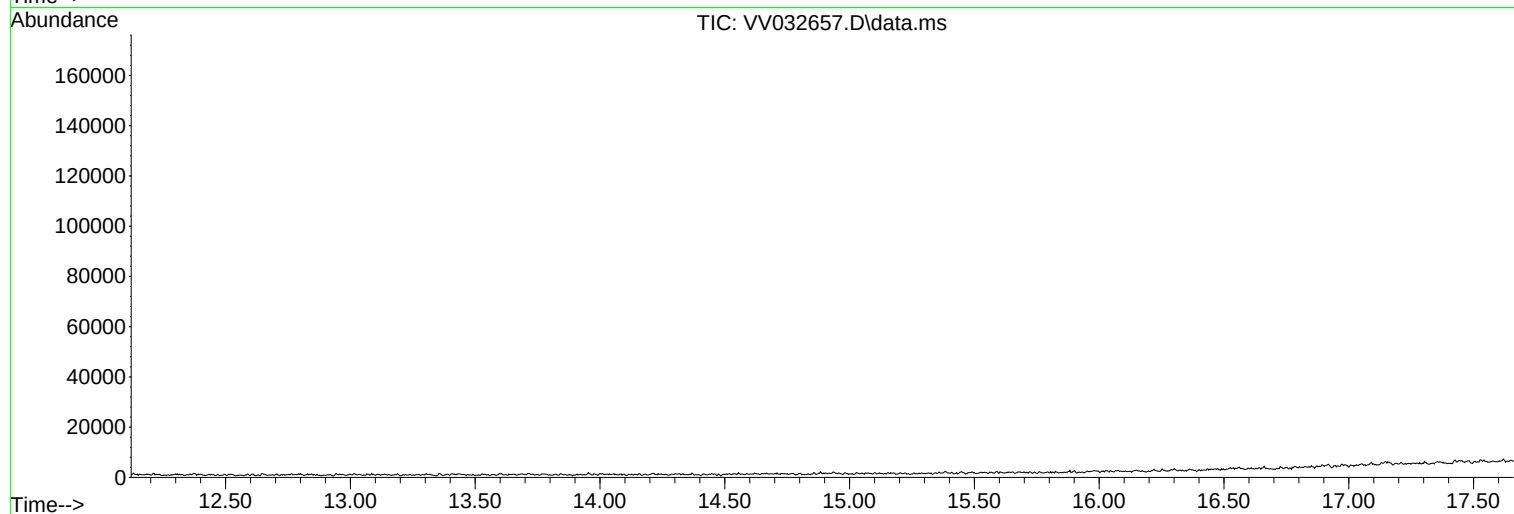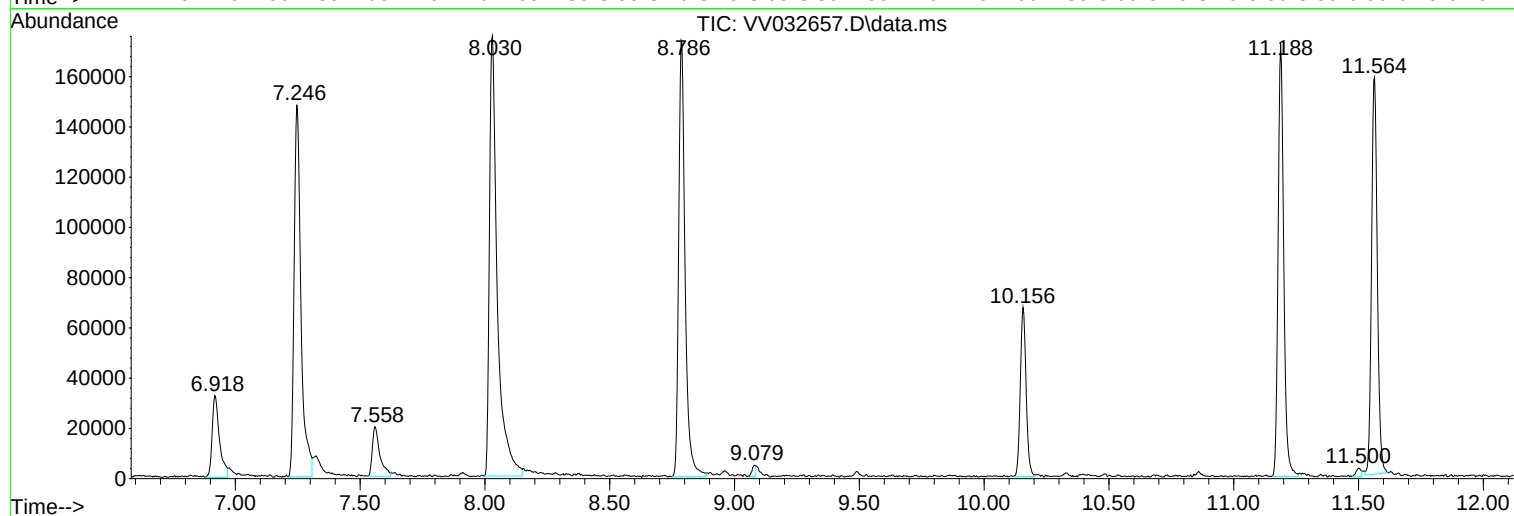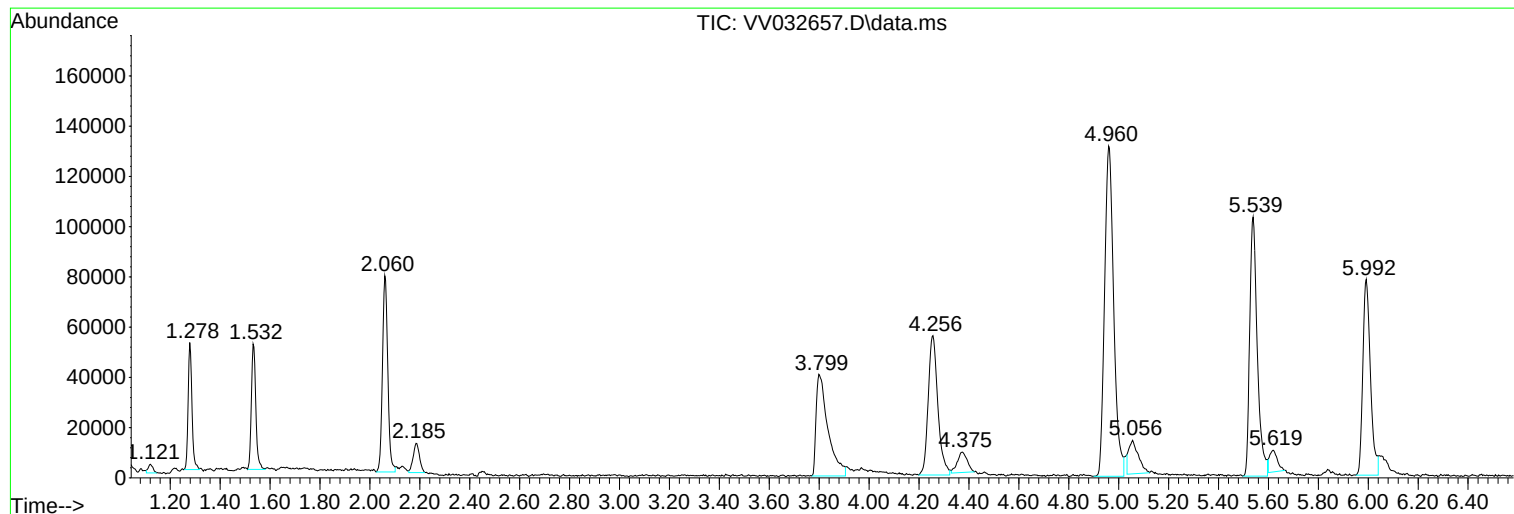

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032657.D
Acq On : 26 Oct 2023 13:04
Operator : SY/MD
Sample : 04995-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032657.D
Acq On : 26 Oct 2023 13:04
Operator : SY/MD
Sample : 04995-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A49L3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------