

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032658.D
 Acq On : 26 Oct 2023 13:29
 Operator : SY/MD
 Sample : 04995-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4A51

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	81	rBV	18017	19162	5.72%	0.927%
2	1.532	146	153	162	rBV	23080	28159	8.40%	1.363%
3	2.060	308	317	326	rBV	24075	35125	10.48%	1.700%
4	2.185	347	356	366	rVB6	4068	7834	2.34%	0.379%
5	2.452	431	439	452	rBV8	4468	8042	2.40%	0.389%
6	3.809	850	861	882	rBV2	34881	113413	33.83%	5.489%
7	4.252	983	999	1023	rBV2	33137	90122	26.89%	4.362%
8	4.368	1024	1035	1050	rVB5	4239	11839	3.53%	0.573%
9	4.960	1203	1219	1239	rBV5	63649	173398	51.73%	8.393%
10	5.539	1387	1399	1414	rBV	93100	195753	58.40%	9.475%
11	5.992	1527	1540	1554	rBV2	46032	99669	29.73%	4.824%
12	6.921	1817	1829	1842	rBV2	18158	36609	10.92%	1.772%
13	7.249	1921	1931	1951	rBV	54299	106436	31.75%	5.152%
14	7.564	2020	2029	2049	rBV2	10813	23941	7.14%	1.159%
15	8.030	2163	2174	2205	rBV	153010	335203	100.00%	16.225%
16	8.786	2397	2409	2432	rBV	158610	283394	84.54%	13.717%
17	10.156	2825	2835	2849	rBV	52696	84436	25.19%	4.087%
18	11.188	3146	3156	3174	rBV	150904	241192	71.95%	11.674%
19	11.500	3246	3253	3257	rBV8	2869	4138	1.23%	0.200%
20	11.564	3262	3273	3291	rVB	89850	147633	44.04%	7.146%
21	12.291	3490	3499	3513	rBV4	12600	20516	6.12%	0.993%




Sum of corrected areas: 2066014

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032658.D
Acq On : 26 Oct 2023 13:29
Operator : SY/MD
Sample : 04995-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

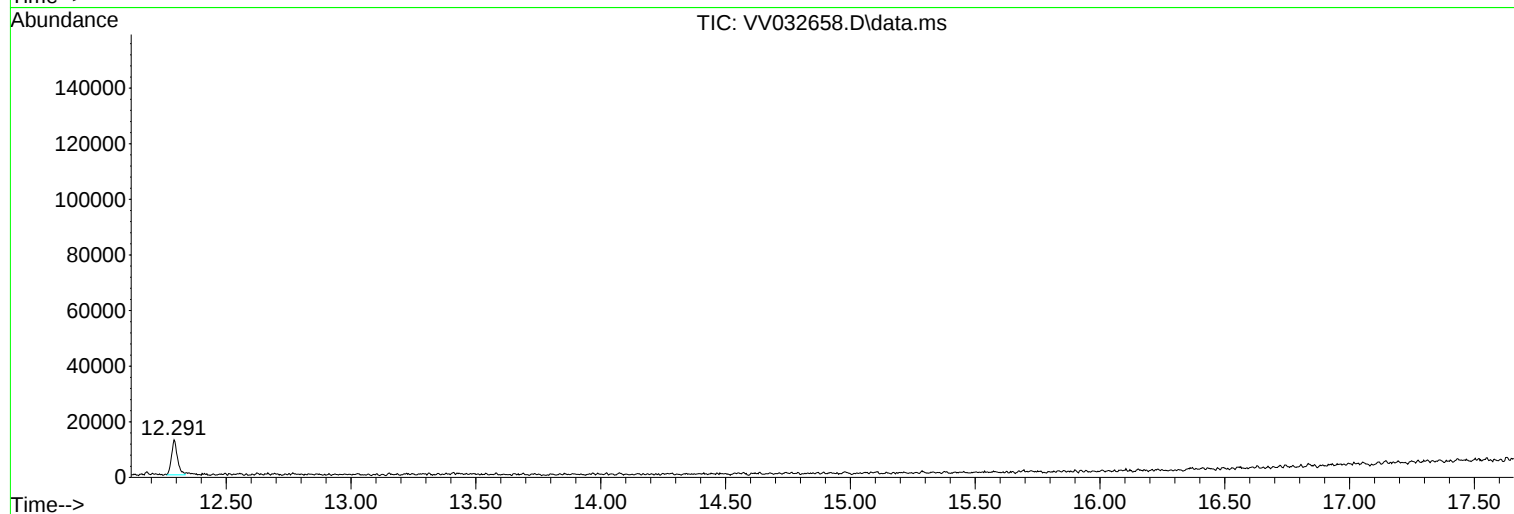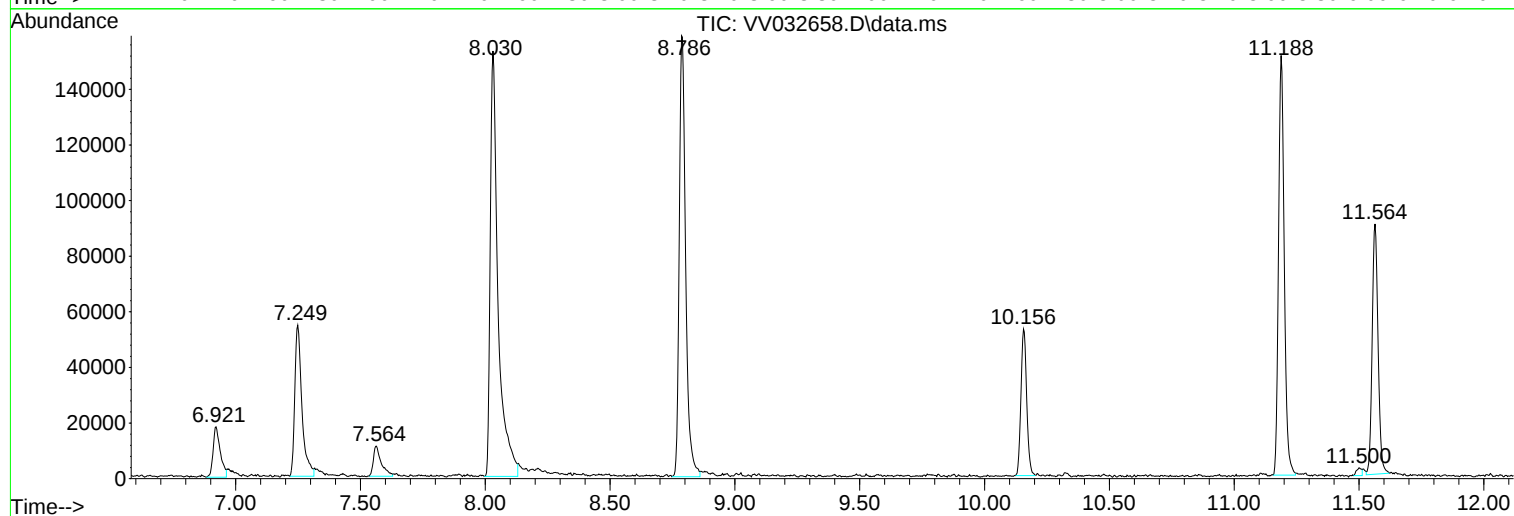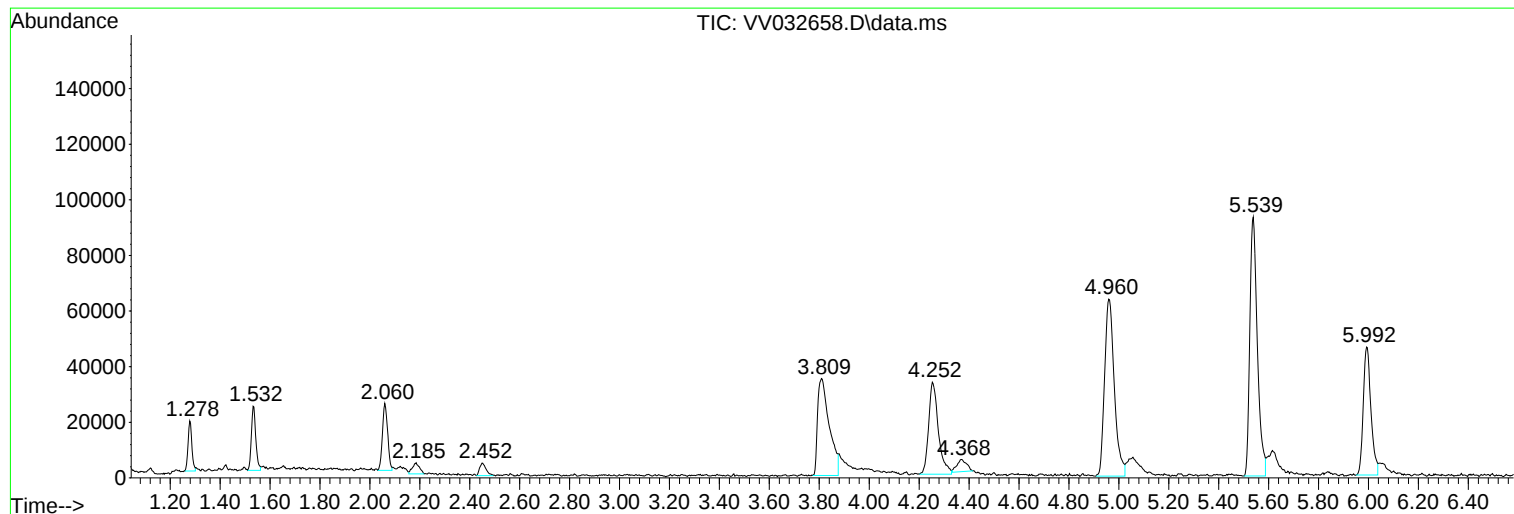

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032658.D
Acq On : 26 Oct 2023 13:29
Operator : SY/MD
Sample : 04995-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032658.D
Acq On : 26 Oct 2023 13:29
Operator : SY/MD
Sample : 04995-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4A51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc