

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032661.D
 Acq On : 26 Oct 2023 14:42
 Operator : SY/MD
 Sample : 05009-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4923

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032661.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	21	26	36	rVB	4062	4842	1.13%	0.141%
2	1.214	49	54	63	rBV2	4230	5809	1.35%	0.169%
3	1.278	67	74	85	rVV	56538	61169	14.23%	1.781%
4	1.532	145	153	165	rBV	57748	69204	16.10%	2.015%
5	2.059	307	317	329	rBV	87440	126790	29.50%	3.691%
6	2.188	348	357	369	rVB2	14369	24796	5.77%	0.722%
7	3.802	849	859	890	rBV2	47057	157512	36.65%	4.586%
8	4.256	984	1000	1023	rBV2	60379	164067	38.18%	4.777%
9	4.378	1023	1038	1057	rVB3	11054	32398	7.54%	0.943%
10	4.960	1203	1219	1238	rBV3	145296	374479	87.14%	10.902%
11	5.053	1239	1248	1275	rVB6	16310	50850	11.83%	1.480%
12	5.538	1388	1399	1415	rBV	106047	222348	51.74%	6.473%
13	5.622	1416	1425	1443	rVB2	9840	27010	6.28%	0.786%
14	5.837	1484	1492	1503	rBV2	2801	5293	1.23%	0.154%
15	5.992	1524	1540	1554	rBV2	89263	188292	43.81%	5.482%
16	6.918	1816	1828	1853	rBV	36956	80949	18.84%	2.357%
17	7.246	1919	1930	1950	rBV	165129	317395	73.85%	9.240%
18	7.561	2017	2028	2050	rBV2	22041	47377	11.02%	1.379%
19	8.027	2161	2173	2207	rBV	200649	429761	100.00%	12.512%
20	8.789	2399	2410	2432	rBV	178434	318517	74.11%	9.273%
21	9.085	2492	2502	2516	rVB5	5328	10309	2.40%	0.300%
22	10.156	2822	2835	2855	rBV	73794	121818	28.35%	3.547%
23	10.857	3044	3053	3064	rBV3	4692	7253	1.69%	0.211%
24	11.188	3145	3156	3179	rVV	172721	277447	64.56%	8.077%
25	11.564	3261	3273	3295	rVB	176546	285481	66.43%	8.311%
26	12.590	3582	3592	3599	rBV10	4925	7824	1.82%	0.228%
27	13.207	3776	3784	3796	rBV5	6351	10347	2.41%	0.301%
28	13.686	3927	3933	3938	rBV4	4472	5540	1.29%	0.161%


Sum of corrected areas: 3434877

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032661.D
Acq On : 26 Oct 2023 14:42
Operator : SY/MD
Sample : 05009-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

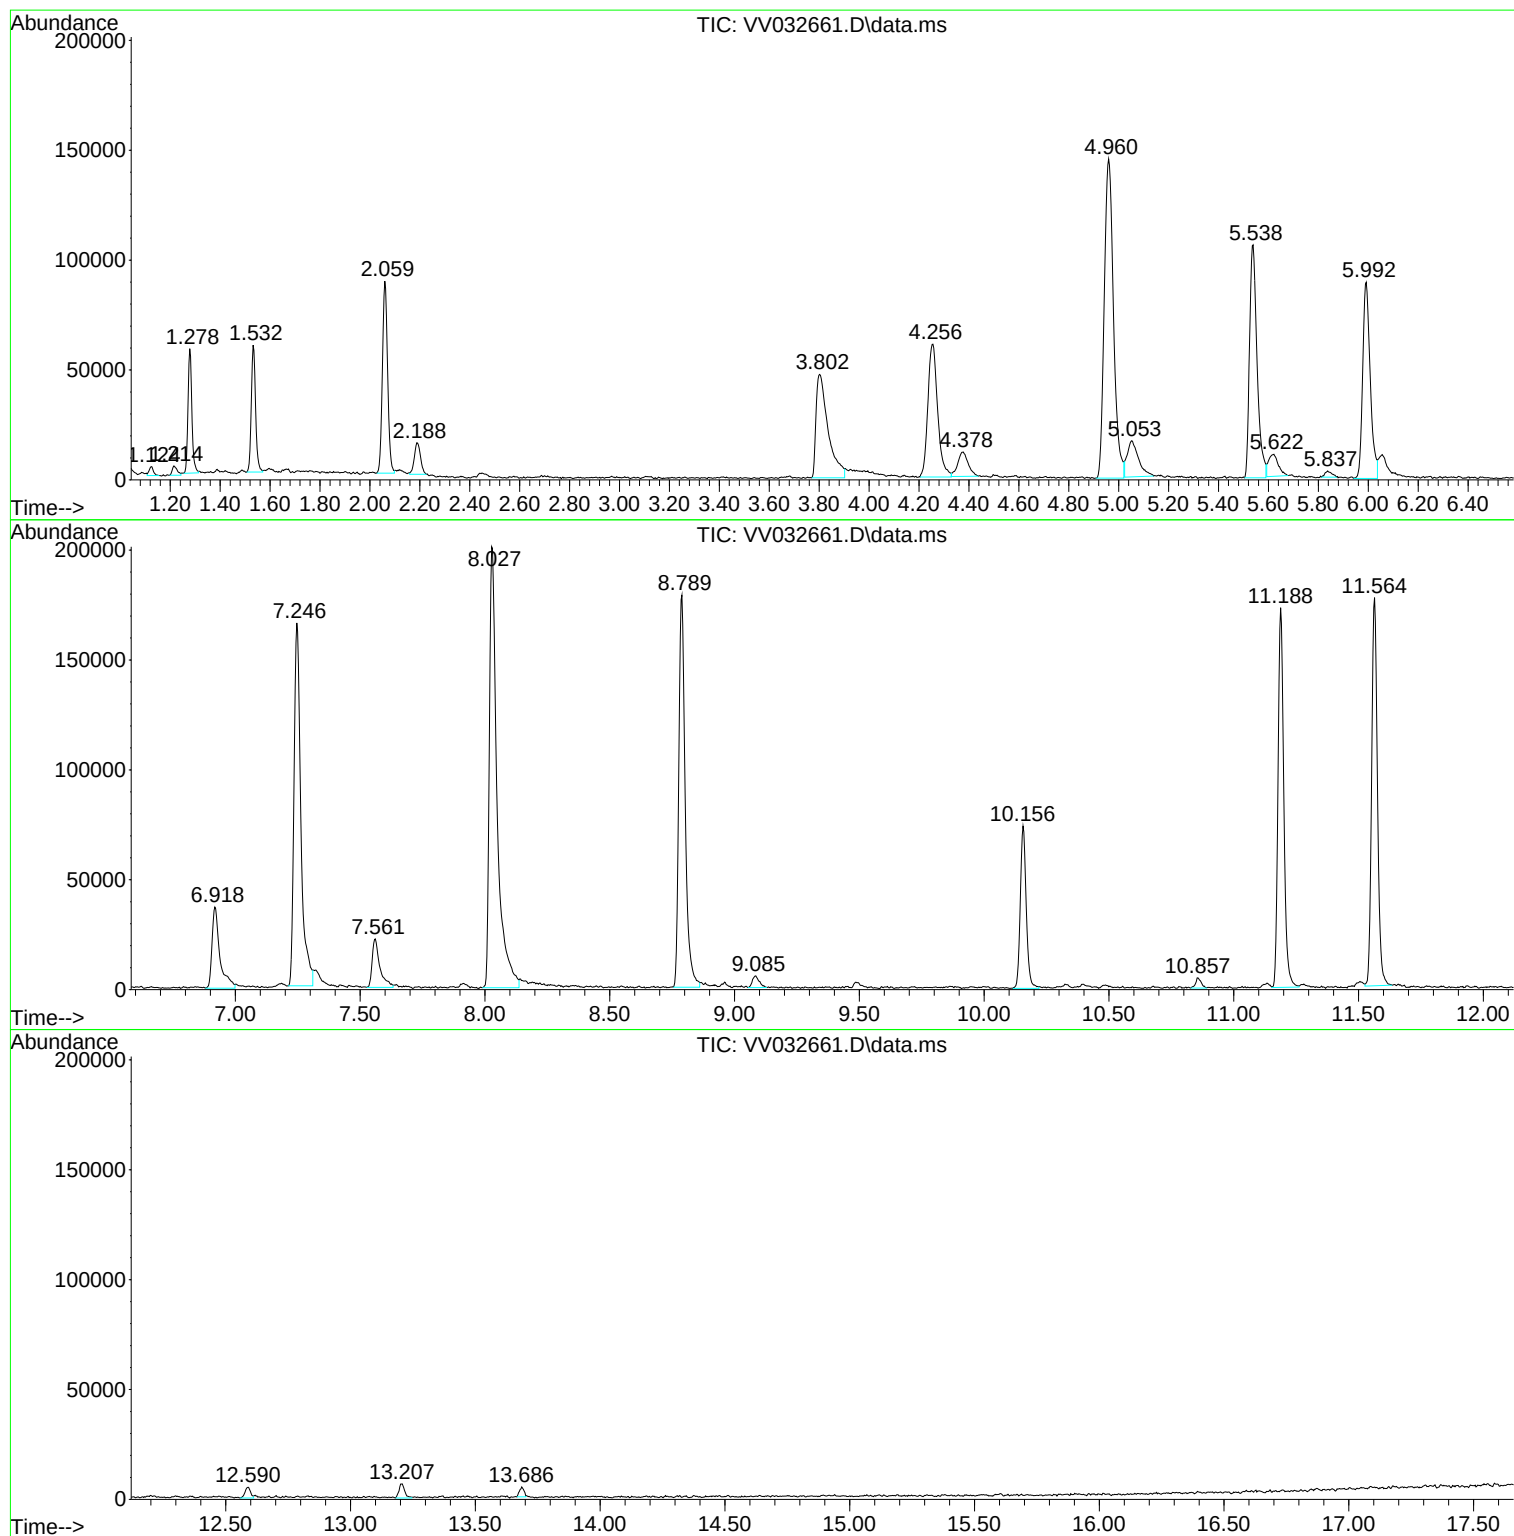

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032661.D
Acq On : 26 Oct 2023 14:42
Operator : SY/MD
Sample : 05009-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032661.D
Acq On : 26 Oct 2023 14:42
Operator : SY/MD
Sample : 05009-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4923

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc