

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032665.D
 Acq On : 26 Oct 2023 16:12
 Operator : SY/MD
 Sample : 05009-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4995

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV032665.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	20	26	35	rVB	3717	4883	1.43%	0.170%
2	1.220	49	56	61	rBV	5057	6757	1.98%	0.236%
3	1.278	67	74	92	rVB	48609	51128	14.96%	1.783%
4	1.532	146	153	166	rVB	48017	58446	17.10%	2.038%
5	2.060	309	317	329	rVB	67386	96441	28.22%	3.363%
6	2.130	334	339	346	rVB7	3102	4829	1.41%	0.168%
7	2.188	349	357	369	rVB2	10342	17798	5.21%	0.621%
8	3.799	846	858	887	rBV	40484	127797	37.39%	4.457%
9	4.252	984	999	1022	rBV2	49887	133801	39.15%	4.666%
10	4.375	1025	1037	1052	rVB2	7784	21054	6.16%	0.734%
11	4.960	1205	1219	1240	rBV3	117317	303884	88.92%	10.598%
12	5.539	1388	1399	1416	rBV	101697	213684	62.52%	7.452%
13	5.619	1417	1424	1439	rVB3	8375	20977	6.14%	0.732%
14	5.992	1527	1540	1555	rBV	72905	154983	45.35%	5.405%
15	6.918	1818	1828	1856	rBV2	28403	64528	18.88%	2.250%
16	7.249	1918	1931	1951	rBV	131418	255329	74.71%	8.904%
17	7.561	2018	2028	2048	rBV	17764	36434	10.66%	1.271%
18	8.030	2164	2174	2203	rBV	160124	341763	100.00%	11.919%
19	8.789	2399	2410	2431	rBV	171248	303277	88.74%	10.577%
20	9.082	2493	2501	2517	rBV3	7021	12620	3.69%	0.440%
21	9.487	2619	2627	2641	rBV9	2798	5180	1.52%	0.181%
22	10.156	2823	2835	2849	rBV	61799	98584	28.85%	3.438%
23	10.326	2880	2888	2897	rVB6	3546	5251	1.54%	0.183%
24	10.860	3046	3054	3063	rBV5	4281	6042	1.77%	0.211%
25	11.188	3145	3156	3177	rBV	166962	271402	79.41%	9.465%
26	11.497	3235	3252	3262	rBV	5328	13590	3.98%	0.474%
27	11.564	3262	3273	3292	rVB	146095	236954	69.33%	8.264%




Sum of corrected areas: 2867416

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032665.D
Acq On : 26 Oct 2023 16:12
Operator : SY/MD
Sample : 05009-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4995

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

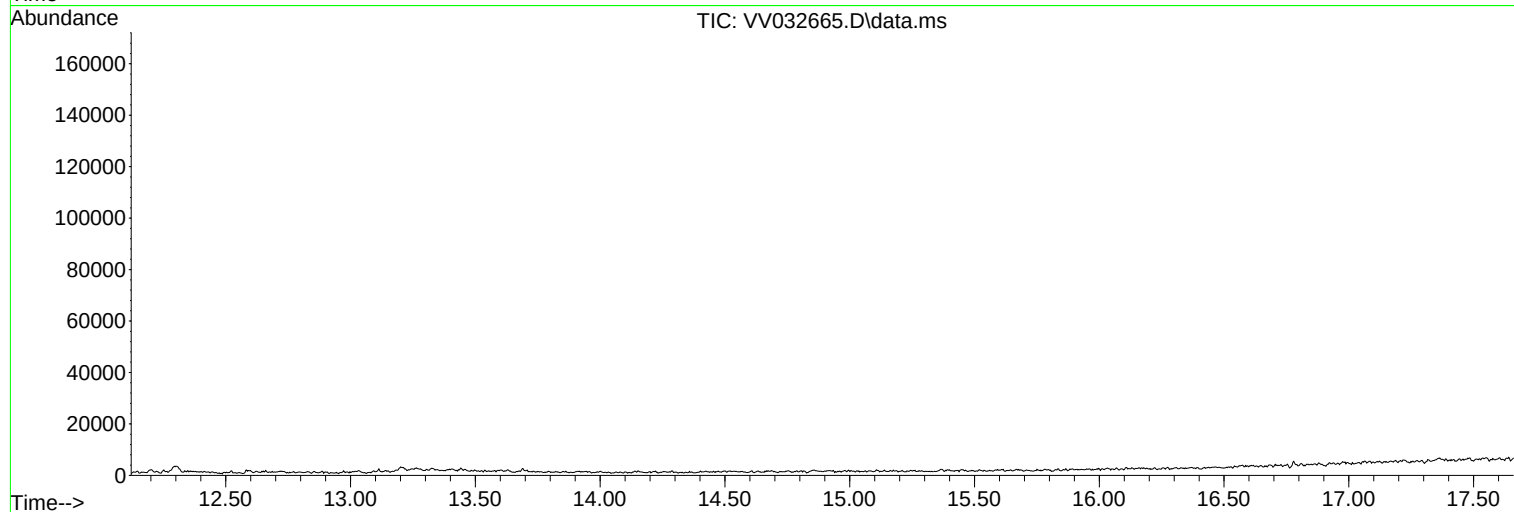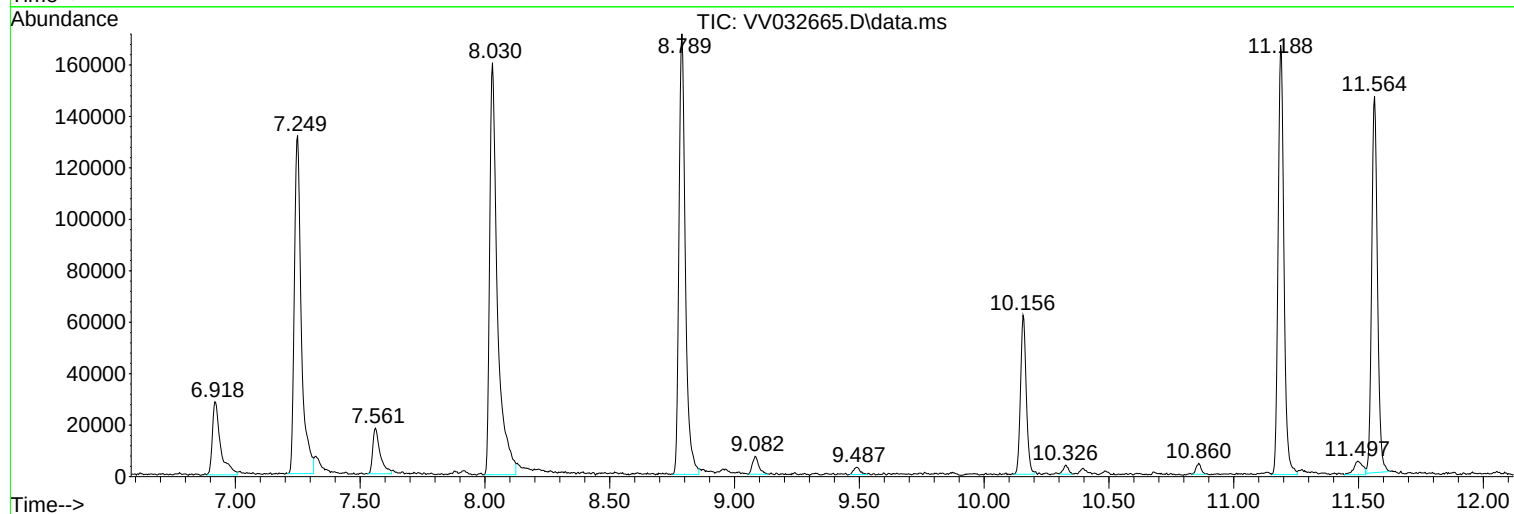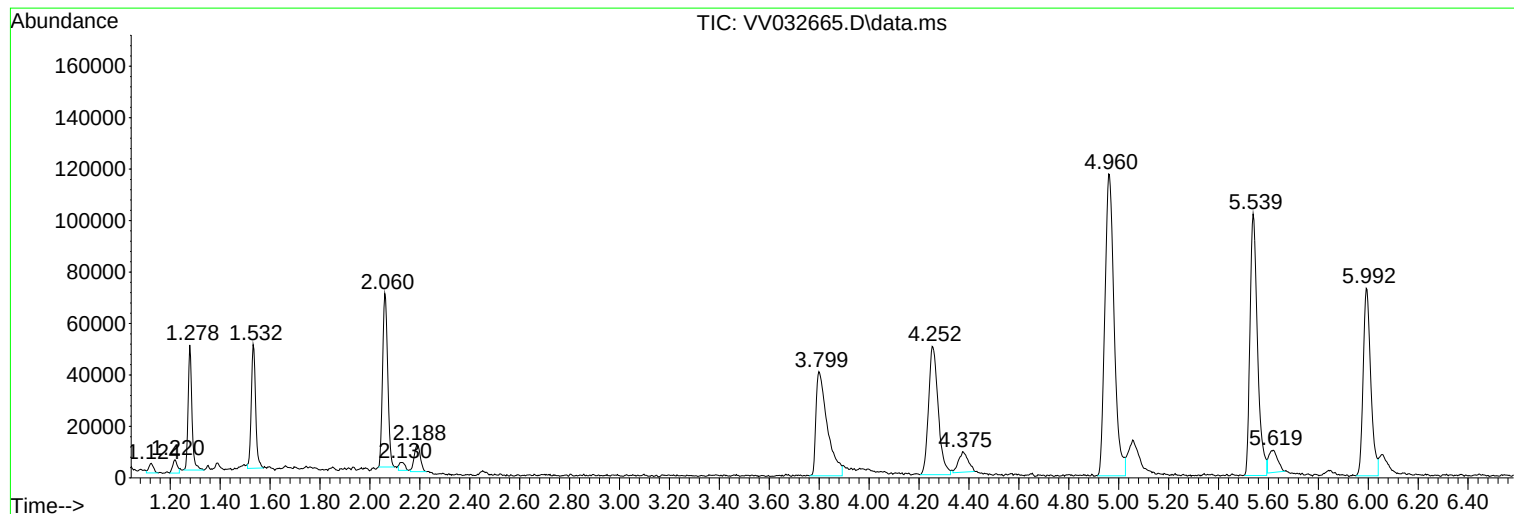

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032665.D
Acq On : 26 Oct 2023 16:12
Operator : SY/MD
Sample : 05009-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4995

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032665.D
Acq On : 26 Oct 2023 16:12
Operator : SY/MD
Sample : 05009-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4995

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc