

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032666.D
 Acq On : 26 Oct 2023 18:02
 Operator : SY/MD
 Sample : 05053-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B16

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032666.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	37	rVB	7714	10093	1.68%	0.287%
2	1.275	66	73	87	rVB	49824	54846	9.13%	1.560%
3	1.529	145	152	163	rVB	45768	54383	9.05%	1.547%
4	2.056	306	316	332	rVB	74563	106149	17.67%	3.019%
5	2.188	349	357	371	rVB3	11521	19623	3.27%	0.558%
6	3.828	855	867	891	rBV	24004	99414	16.55%	2.828%
7	4.252	982	999	1020	rBV2	47927	125329	20.86%	3.565%
8	4.375	1024	1037	1056	rVB3	10530	27636	4.60%	0.786%
9	4.957	1202	1218	1237	rBV3	117827	297827	49.58%	8.471%
10	5.056	1239	1249	1268	rVB6	13202	39762	6.62%	1.131%
11	5.535	1384	1398	1416	rBV	104333	220878	36.77%	6.282%
12	5.619	1417	1424	1442	rVB3	11284	28304	4.71%	0.805%
13	5.992	1526	1540	1555	rBV2	68463	149552	24.90%	4.254%
14	6.053	1556	1559	1572	rVB7	7490	14129	2.35%	0.402%
15	6.918	1818	1828	1839	rBV2	28077	54611	9.09%	1.553%
16	7.246	1919	1930	1966	rBV	137344	269053	44.79%	7.653%
17	7.561	2019	2028	2041	rBV2	17618	34945	5.82%	0.994%
18	7.905	2120	2135	2162	rBV	322745	600728	100.00%	17.086%
19	8.034	2165	2175	2211	rBV	154111	356135	59.28%	10.130%
20	8.789	2394	2410	2430	rBV	175264	314599	52.37%	8.948%
21	10.156	2823	2835	2851	rBV	60383	100360	16.71%	2.855%
22	11.188	3146	3156	3179	rVB	169096	272983	45.44%	7.764%
23	11.564	3262	3273	3291	rVB	141766	229752	38.25%	6.535%
24	13.201	3774	3782	3796	rBV4	6211	10154	1.69%	0.289%
25	13.445	3849	3858	3868	rBV2	8356	13578	2.26%	0.386%
26	13.686	3922	3933	3943	rBV4	7044	10996	1.83%	0.313%




Sum of corrected areas: 3515819

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032666.D
Acq On : 26 Oct 2023 18:02
Operator : SY/MD
Sample : 05053-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

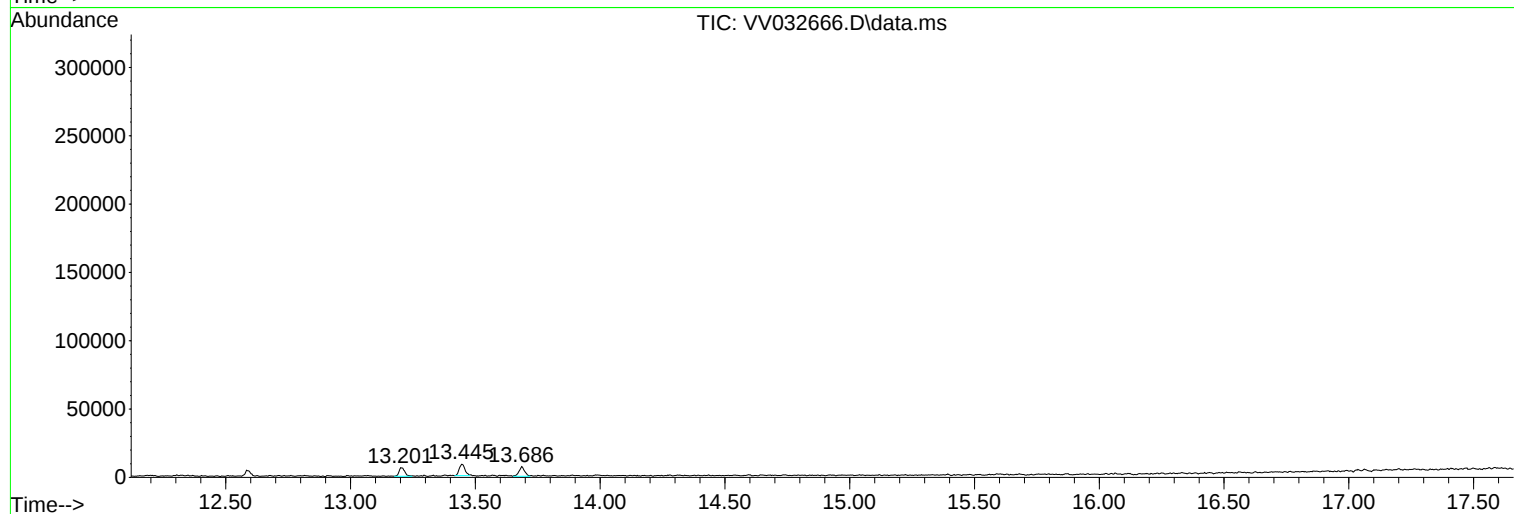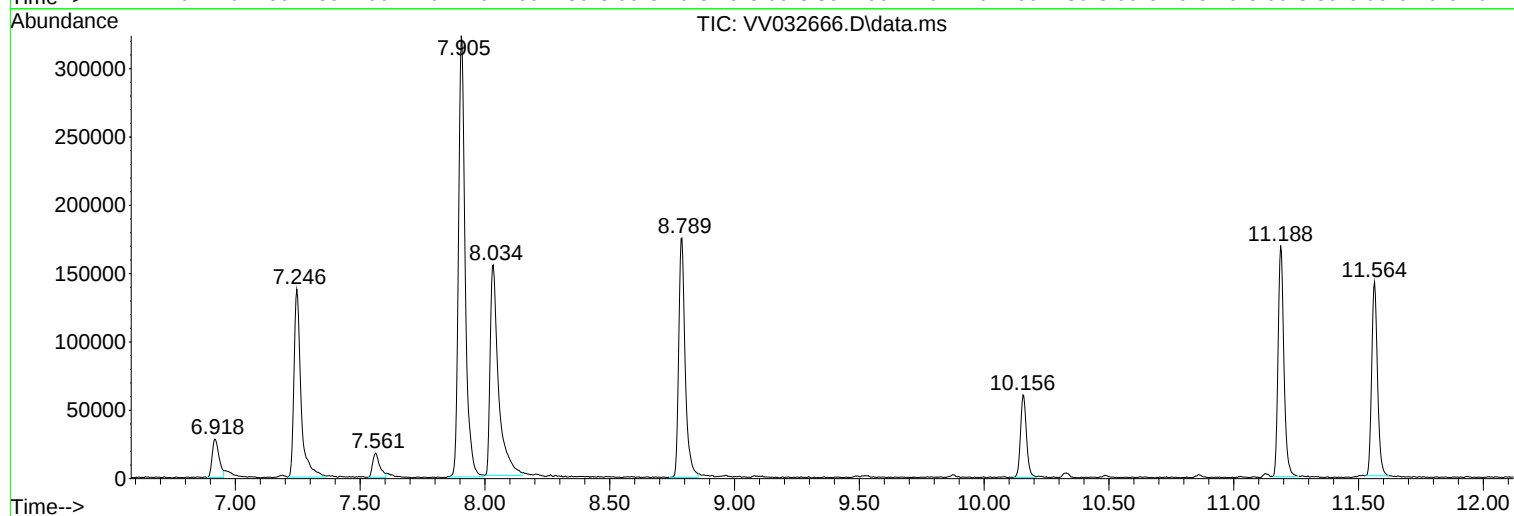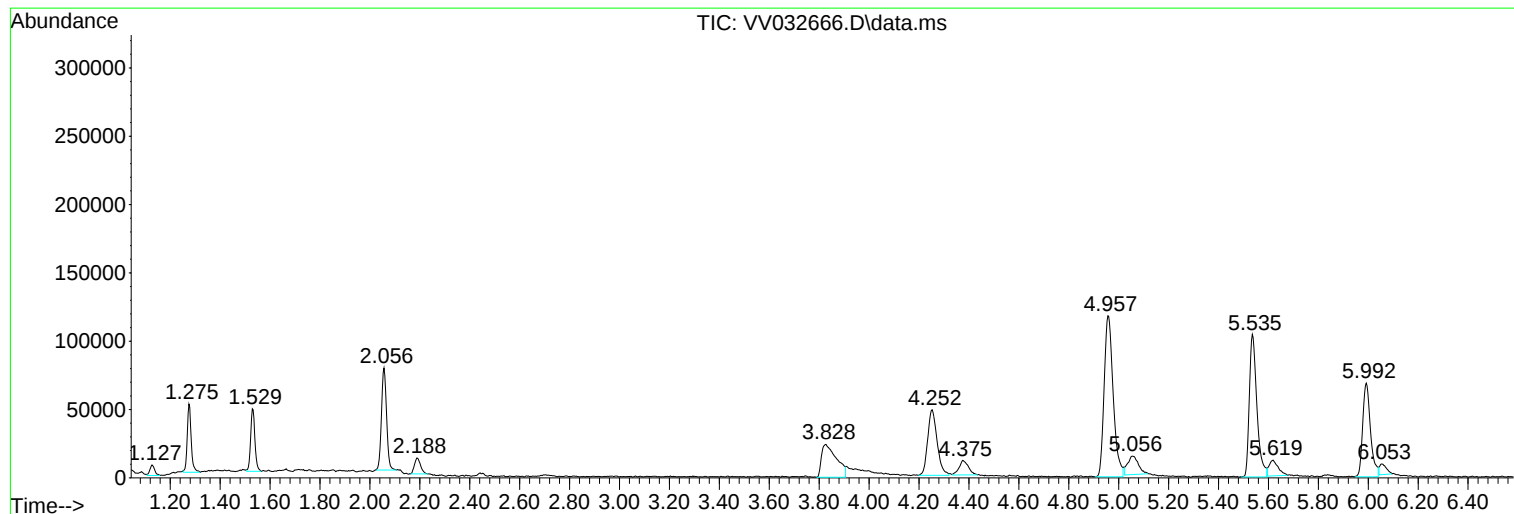

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032666.D
Acq On : 26 Oct 2023 18:02
Operator : SY/MD
Sample : 05053-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032666.D
Acq On : 26 Oct 2023 18:02
Operator : SY/MD
Sample : 05053-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B16

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc