

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032667.D
 Acq On : 26 Oct 2023 18:26
 Operator : SY/MD
 Sample : 05053-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B17

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032667.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.130	22	28	38	rVB	5106	6786	1.81%	0.227%
2	1.278	65	74	85	rBV	50077	53801	14.32%	1.801%
3	1.532	146	153	167	rVB	48254	57415	15.29%	1.922%
4	2.060	308	317	331	rVB	73368	105203	28.01%	3.522%
5	2.195	348	359	370	rBV2	12459	22717	6.05%	0.760%
6	3.805	852	860	879	rBV	26161	78406	20.87%	2.625%
7	4.252	985	999	1020	rBV	50163	128865	34.31%	4.314%
8	4.384	1027	1040	1055	rVB2	10092	27063	7.20%	0.906%
9	4.960	1203	1219	1238	rBV3	123739	316934	84.38%	10.609%
10	5.056	1240	1249	1274	rVB4	13691	41388	11.02%	1.385%
11	5.539	1386	1399	1417	rBV	101059	214543	57.12%	7.182%
12	5.619	1417	1424	1435	rVB	7547	16791	4.47%	0.562%
13	5.992	1528	1540	1556	rBV	75281	158901	42.30%	5.319%
14	6.445	1672	1681	1691	rBV6	3345	5859	1.56%	0.196%
15	6.918	1817	1828	1839	rBV	29659	56369	15.01%	1.887%
16	7.246	1919	1930	1957	rBV	141670	276739	73.68%	9.264%
17	7.561	2019	2028	2043	rBV2	17969	37843	10.07%	1.267%
18	7.908	2113	2136	2155	rBV4	19602	46119	12.28%	1.544%
19	8.030	2163	2174	2213	rBV	149874	375615	100.00%	12.573%
20	8.185	2213	2222	2233	rVB4	9188	19785	5.27%	0.662%
21	8.789	2397	2410	2430	rBV	170474	305164	81.24%	10.215%
22	9.677	2676	2686	2694	rBV9	3811	6453	1.72%	0.216%
23	10.156	2825	2835	2856	rVB2	64607	107870	28.72%	3.611%
24	10.329	2876	2889	2899	rBV2	6240	10406	2.77%	0.348%
25	11.188	3144	3156	3175	rBV	164011	263988	70.28%	8.837%
26	11.564	3261	3273	3288	rVV	151354	242294	64.51%	8.111%
27	13.448	3849	3859	3867	rBV7	2836	4080	1.09%	0.137%




Sum of corrected areas: 2987397

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032667.D
Acq On : 26 Oct 2023 18:26
Operator : SY/MD
Sample : 05053-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

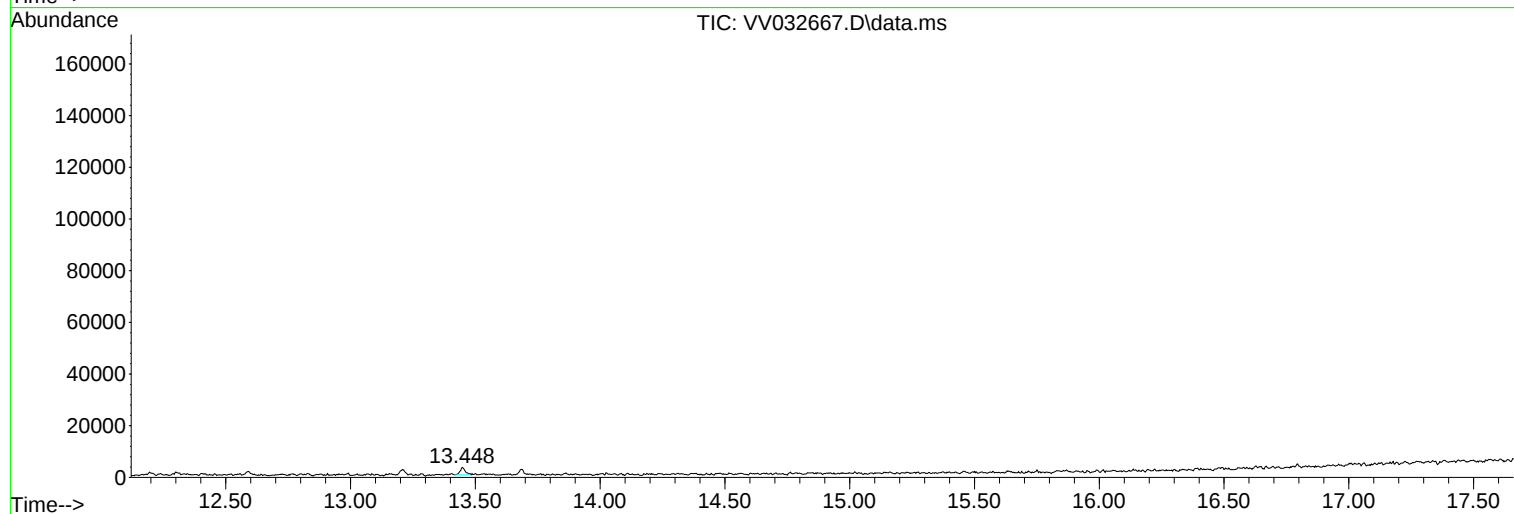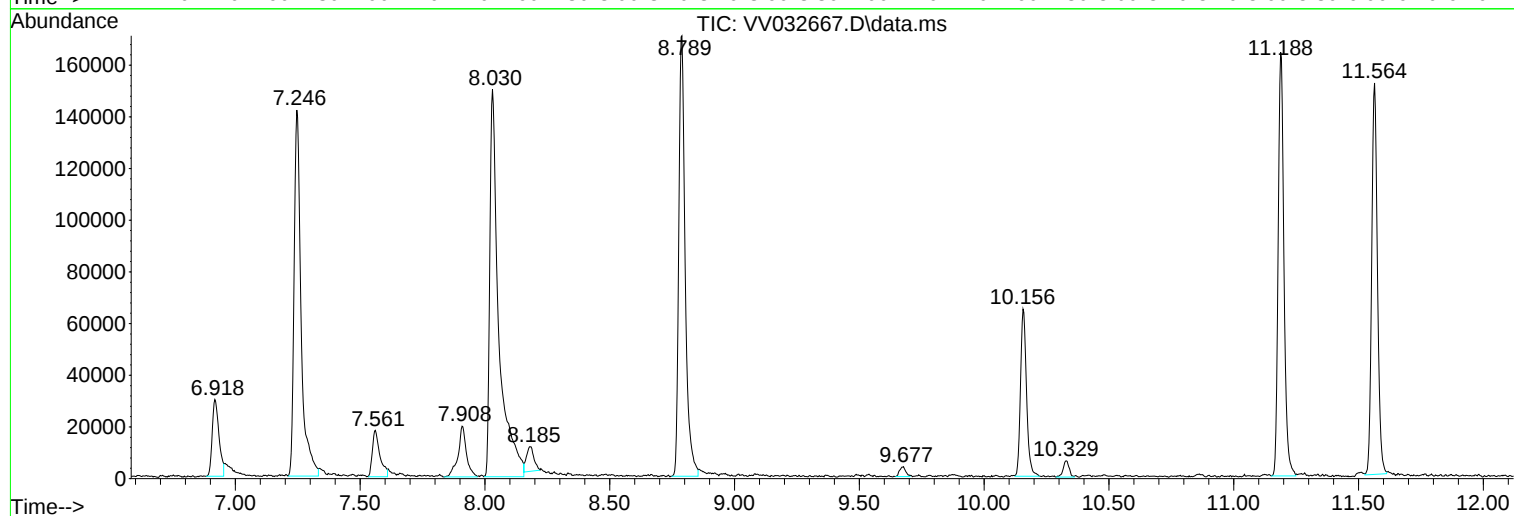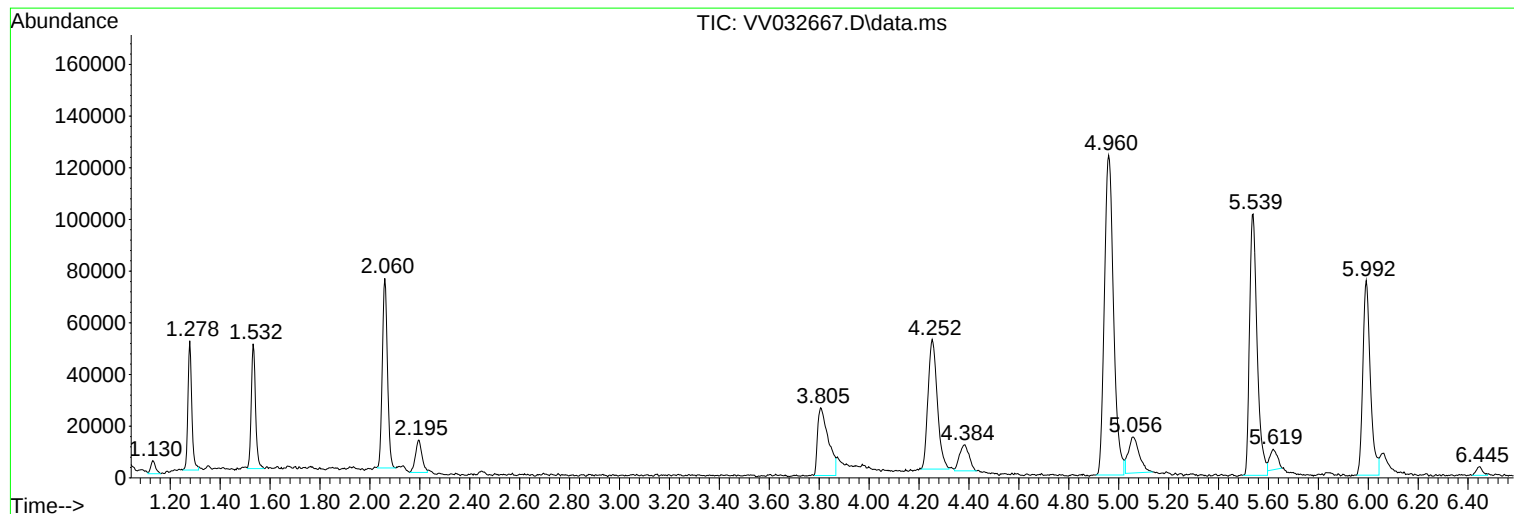

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032667.D
Acq On : 26 Oct 2023 18:26
Operator : SY/MD
Sample : 05053-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032667.D
Acq On : 26 Oct 2023 18:26
Operator : SY/MD
Sample : 05053-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc