

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
 Data File : VV032669.D
 Acq On : 26 Oct 2023 19:15
 Operator : SY/MD
 Sample : 05053-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0B20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV032669.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.127	21	27	35	rVB	4373	5670	1.62%	0.199%
2	1.278	67	74	88	rBV	46709	49875	14.25%	1.754%
3	1.532	145	153	167	rVB	45973	54819	15.66%	1.928%
4	2.060	307	317	331	rBV	67893	101748	29.07%	3.579%
5	2.191	348	358	373	rVB2	12045	21476	6.14%	0.755%
6	3.809	852	861	888	rBV2	22959	79461	22.70%	2.795%
7	4.256	985	1000	1018	rBV	47664	125766	35.93%	4.424%
8	4.378	1028	1038	1061	rVB2	9918	28726	8.21%	1.010%
9	4.960	1203	1219	1237	rBV2	117701	298907	85.39%	10.514%
10	5.056	1243	1249	1267	rVB7	11436	28609	8.17%	1.006%
11	5.535	1387	1398	1416	rBV	98402	209051	59.72%	7.353%
12	5.619	1417	1424	1436	rVB3	7604	17635	5.04%	0.620%
13	5.992	1528	1540	1555	rBV2	70311	150960	43.13%	5.310%
14	6.442	1671	1680	1687	rBV4	3296	6108	1.74%	0.215%
15	6.918	1818	1828	1842	rBV	28362	56343	16.10%	1.982%
16	7.246	1918	1930	1956	rBV	132473	257923	73.69%	9.072%
17	7.561	2020	2028	2043	rBV	17330	33611	9.60%	1.182%
18	7.908	2114	2136	2156	rVB4	17636	40488	11.57%	1.424%
19	8.030	2164	2174	2212	rBV	136376	350029	100.00%	12.312%
20	8.182	2214	2221	2243	rVB5	10424	24491	7.00%	0.861%
21	8.786	2398	2409	2432	rBV	166945	297472	84.98%	10.463%
22	9.674	2678	2685	2695	rVB5	3594	6382	1.82%	0.224%
23	10.156	2825	2835	2852	rBV	60105	99883	28.54%	3.513%
24	10.326	2880	2888	2897	rBV3	3635	6250	1.79%	0.220%
25	11.188	3145	3156	3172	rBV	161724	257539	73.58%	9.059%
26	11.519	3248	3259	3262	rBV7	1920	3750	1.07%	0.132%
27	11.564	3262	3273	3293	rVV	138551	229985	65.70%	8.090%




Sum of corrected areas: 2842957

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032669.D
Acq On : 26 Oct 2023 19:15
Operator : SY/MD
Sample : 05053-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

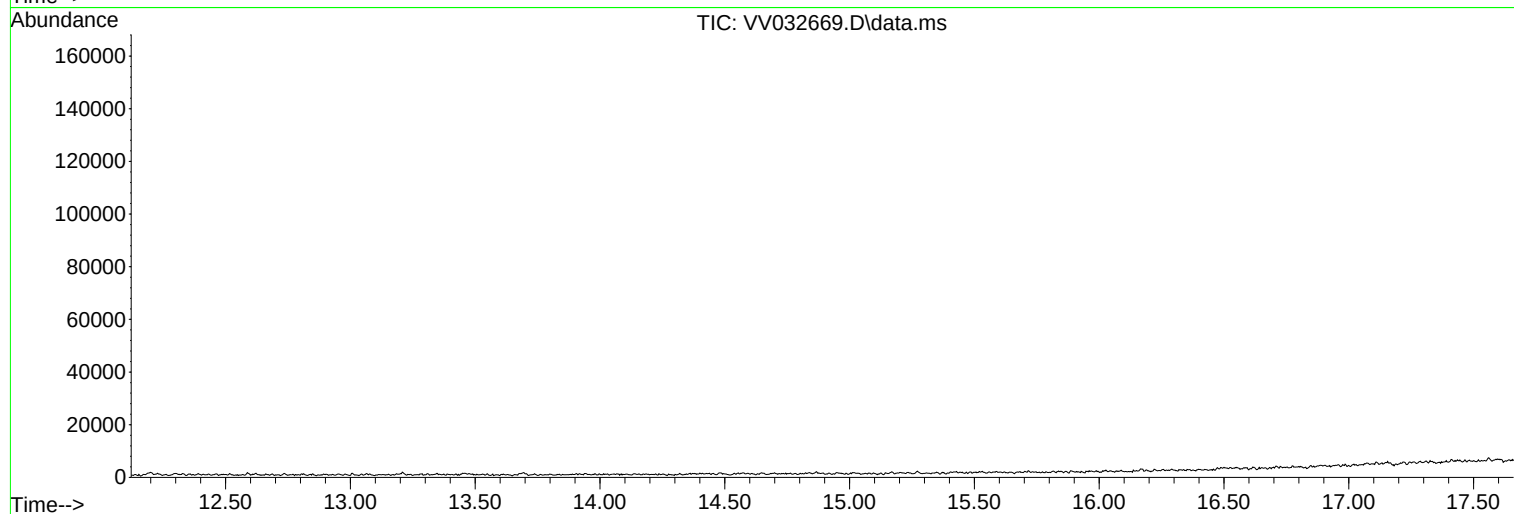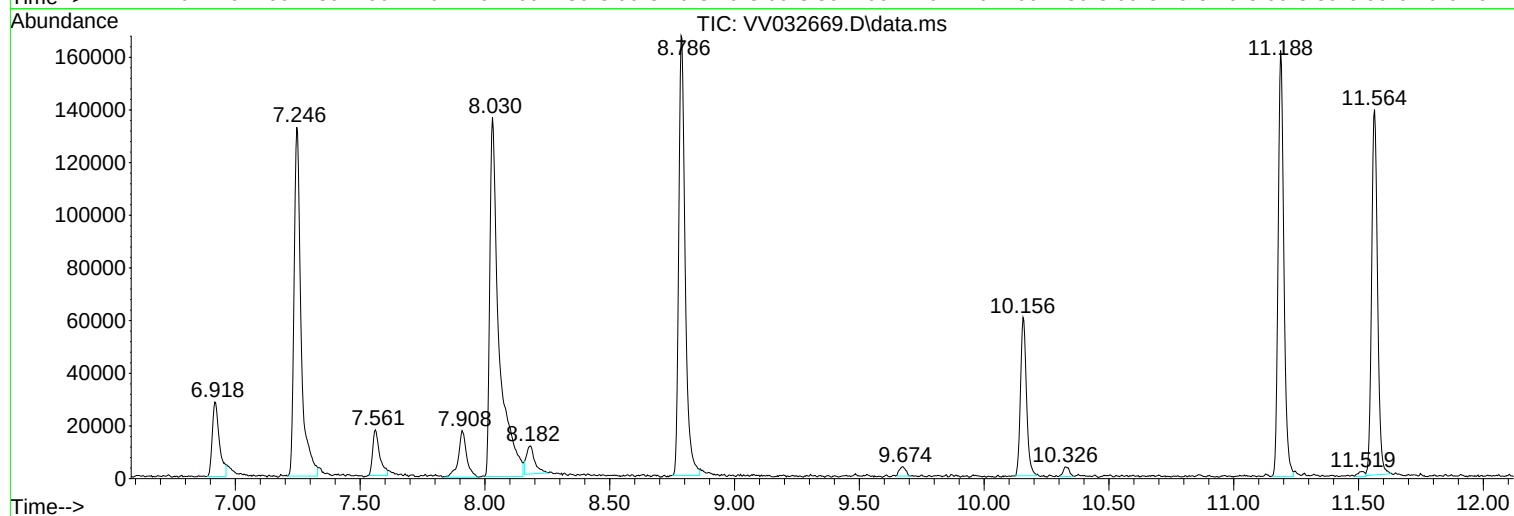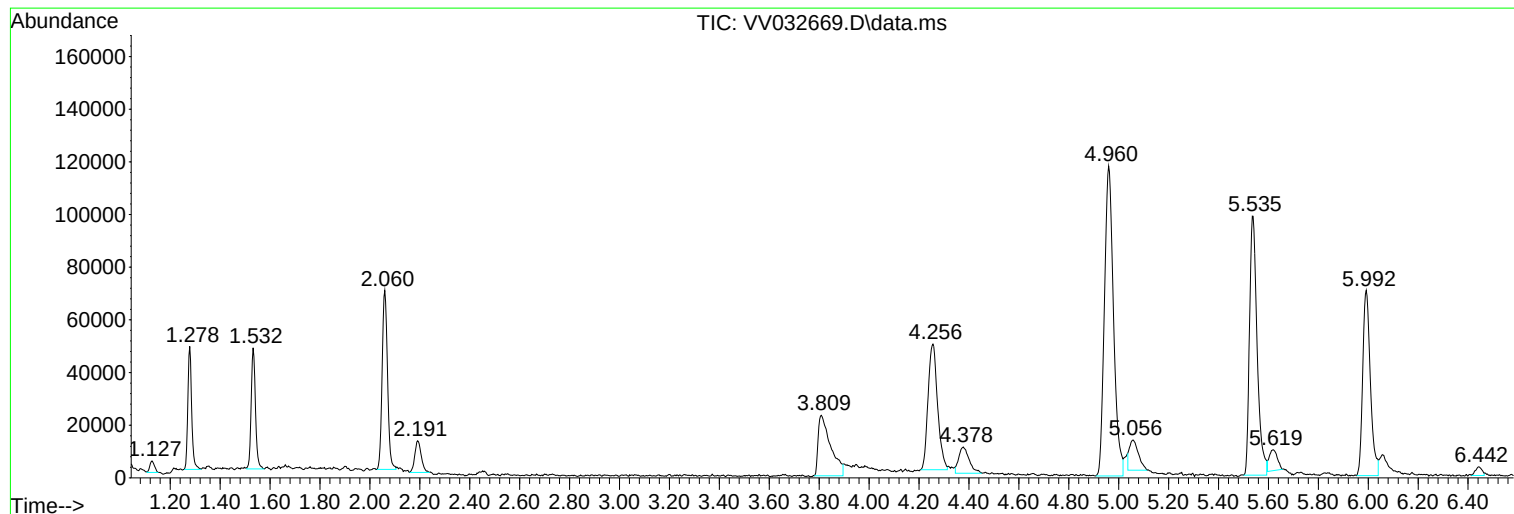

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032669.D
Acq On : 26 Oct 2023 19:15
Operator : SY/MD
Sample : 05053-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032669.D
Acq On : 26 Oct 2023 19:15
Operator : SY/MD
Sample : 05053-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0B20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc