
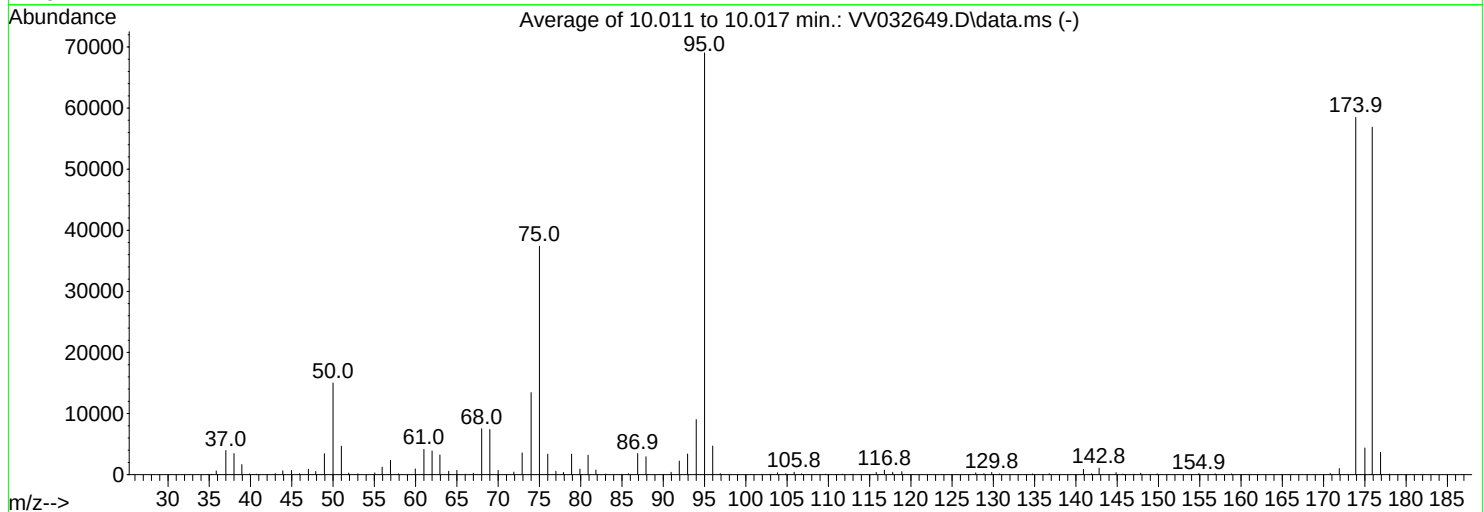


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102623\
Data File : VV032649.D
Acq On : 26 Oct 2023 08:32
Operator : SY/MD
Sample : BFB228
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB228

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR092923WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Oct 27 05:30:38 2023

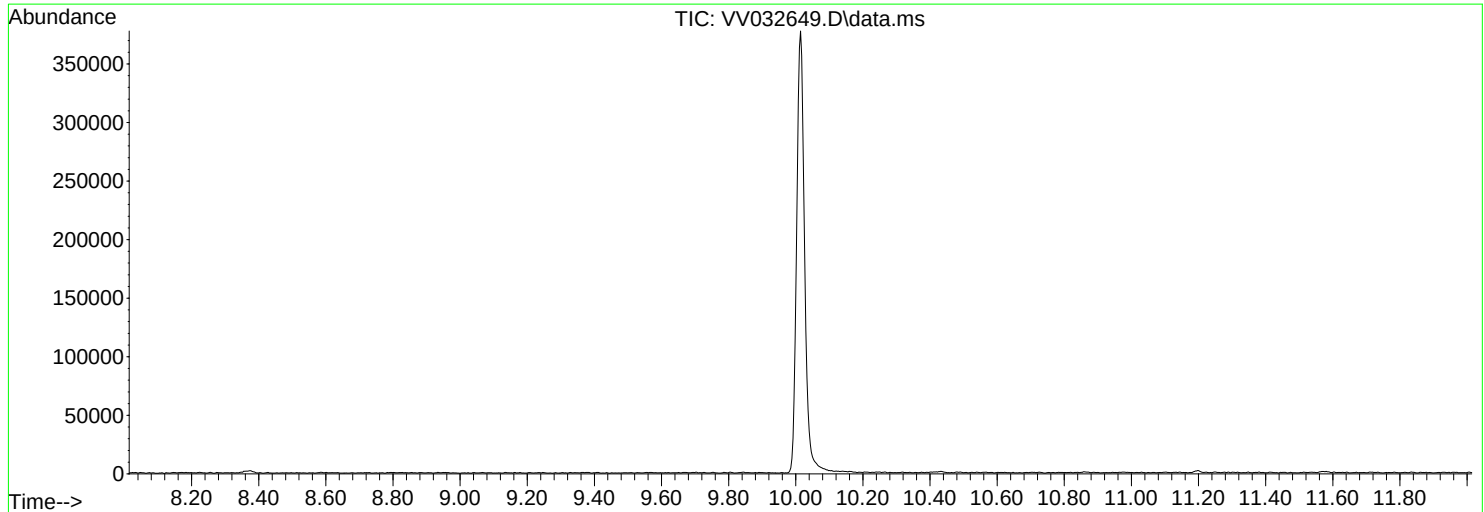

AutoFind: Scans 2790, 2791, 2792; Background Corrected with Scan 2778

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	15010	PASS
75	95	30	80	54.2	37400	PASS
95	95	100	100	100.0	69040	PASS
96	95	5	9	6.8	4678	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	84.7	58493	PASS
175	174	5	9	7.5	4376	PASS
176	174	95	105	97.3	56899	PASS
177	176	5	10	6.4	3648	PASS

m/z	Abundance
35.90	185.0
38.10	120.0
40.00	166.0
43.90	296.0
48.70	105.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.90	868.0
37.00	4031.0
38.00	3660.0
38.90	1575.0
39.90	263.0
42.90	170.0
43.90	918.0
44.90	717.0
45.90	164.0
47.00	908.0
47.90	538.0
49.00	3621.0
50.00	15249.0
51.00	4958.0
51.90	244.0
53.00	132.0
55.00	276.0
55.90	1228.0
56.90	2292.0
58.00	148.0
60.00	972.0
61.00	4239.0
62.00	3923.0
62.90	3207.0
64.00	582.0
65.00	722.0
66.00	115.0
67.00	204.0
68.00	7286.0
69.00	7267.0
70.00	724.0
71.90	447.0
72.90	3486.0
74.00	13478.0
75.00	37680.0
76.00	3436.0
77.00	558.0
77.90	377.0
78.90	3455.0
79.90	867.0
80.90	3243.0
81.90	764.0
83.00	107.0
85.80	186.0
86.90	3466.0
87.90	2937.0
90.90	345.0
92.00	2200.0
92.90	3381.0
94.00	8800.0
95.00	69056.0
96.00	4828.0
96.90	174.0
102.90	130.0
103.80	335.0
104.90	151.0
105.80	385.0
106.80	133.0
109.70	110.0
110.90	105.0
113.00	116.0
114.70	115.0
115.80	411.0
116.80	795.0
117.80	370.0
118.90	467.0
125.60	102.0
127.80	280.0
128.90	189.0
129.80	333.0
130.70	118.0
134.70	137.0
136.70	156.0
140.90	910.0
141.90	114.0
142.80	1043.0
144.90	346.0
145.70	151.0
147.80	231.0
149.80	124.0
154.90	196.0
156.90	149.0
158.90	132.0
170.80	211.0
171.90	924.0
173.90	56208.0
175.00	4470.0
175.90	55552.0
176.90	3580.0
177.90	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.90	808.0
37.00	4093.0
38.00	3670.0
39.00	1729.0
39.90	292.0
40.70	103.0
43.00	174.0
43.90	933.0
44.90	708.0
45.90	175.0
47.00	905.0
47.90	549.0
49.00	3521.0
50.00	15537.0
51.00	4791.0
51.90	268.0
53.00	128.0
55.00	281.0
55.90	1265.0
56.90	2414.0
58.00	145.0
59.90	981.0
61.00	4297.0
62.00	3929.0
62.90	3321.0
64.00	565.0
65.00	739.0
66.00	125.0
67.00	234.0
68.00	7768.0
69.00	7533.0
70.00	738.0
71.90	439.0
72.90	3659.0
74.00	13922.0
75.00	38632.0
76.00	3423.0
77.00	584.0
77.90	383.0
78.90	3472.0
79.90	946.0
80.90	3249.0
81.90	796.0
83.10	115.0
85.80	159.0
86.90	3599.0
87.90	3094.0
91.00	390.0
91.90	2327.0
93.00	3484.0
94.00	9254.0
95.00	71280.0
96.00	4779.0
96.90	171.0
103.00	130.0
103.80	304.0
104.80	161.0
105.90	402.0
106.80	123.0
109.70	114.0
111.70	115.0
113.00	101.0
115.80	397.0
116.80	751.0
117.80	426.0
118.90	524.0
127.80	286.0
128.90	189.0
129.80	375.0
130.80	132.0
134.70	144.0
136.80	150.0
140.90	877.0
141.90	166.0
142.80	1061.0
144.80	375.0
145.70	142.0
147.00	102.0
147.80	236.0
149.90	129.0
154.90	195.0
156.80	146.0
158.90	132.0
170.80	206.0
171.90	1016.0
173.90	60456.0
175.00	4423.0
175.90	58912.0
176.90	3728.0
177.90	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228

m/z	Abundance
35.30	143.0
35.90	678.0
37.00	3770.0
38.00	3380.0
39.00	1683.0
39.90	292.0
40.70	110.0
43.10	148.0
43.90	912.0
45.00	631.0
46.00	166.0
47.00	875.0
47.90	523.0
48.90	3165.0
50.00	14244.0
51.00	4214.0
51.90	282.0
53.00	136.0
55.10	293.0
56.00	1210.0
57.00	2273.0
57.90	145.0
60.00	890.0
61.00	3909.0
62.00	3744.0
63.00	3114.0
64.00	499.0
65.00	681.0
67.00	245.0
68.00	7519.0
69.00	7362.0
70.00	674.0
71.90	405.0
72.90	3559.0
74.00	12922.0
75.00	35888.0
76.00	3214.0
77.00	522.0
77.90	357.0
78.90	3126.0
79.90	936.0
80.90	3110.0
81.80	728.0
83.10	102.0
85.80	108.0
86.90	3332.0
87.90	2811.0
91.00	435.0
91.90	2147.0
93.00	3284.0
94.00	8987.0
95.00	66784.0
96.00	4427.0
96.90	144.0
103.90	279.0
104.80	165.0
105.90	388.0
106.70	113.0
111.70	103.0
112.70	102.0
115.80	326.0
116.80	677.0
117.80	417.0
118.90	507.0
127.90	303.0
128.80	149.0
129.80	368.0
130.80	152.0
134.80	157.0
136.80	146.0
140.90	801.0
141.90	187.0
142.80	1095.0
144.80	277.0
145.90	105.0
147.10	111.0
147.90	223.0
149.90	121.0
154.90	183.0
156.80	158.0
158.80	121.0
170.80	151.0
171.90	1012.0
173.90	58816.0
175.00	4236.0
175.90	56232.0
176.90	3636.0
178.00	115.0

Instrument :
MSVOA_V
ClientSampleId :
BFB228