


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV102720\
Data File : VV019125.D
Acq On : 27 Oct 2020 08:59
Operator : SY/MD
Sample : BFB83
Misc : 5.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB83

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM102220WMA.M
Title : VOC Analysis
Last Update : Wed Oct 28 01:06:58 2020

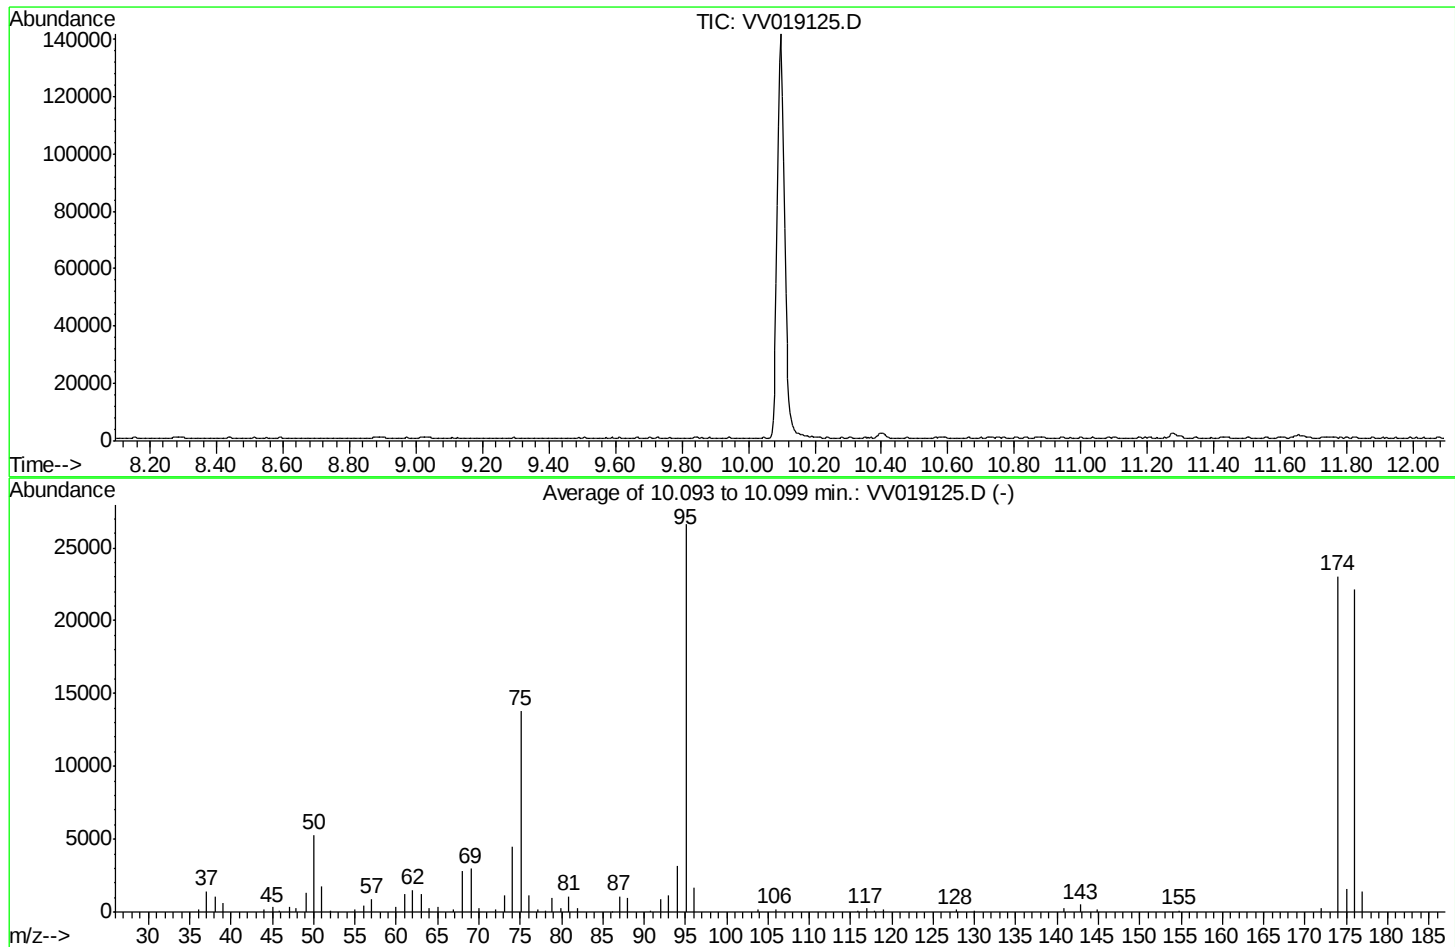

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2790

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	5284	PASS
75	95	30	80	51.9	13818	PASS
95	95	100	100	100.0	26610	PASS
96	95	5	9	6.2	1640	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	86.6	23037	PASS
175	174	5	9	6.9	1592	PASS
176	174	95	101	96.2	22173	PASS
177	176	5	9	6.4	1421	PASS

m/z	Abundance
36.00	227.0
37.00	1395.0
38.10	1084.0
39.00	594.0
39.90	120.0
44.00	1000.0
45.00	303.0
45.90	124.0
47.00	394.0
47.90	240.0
49.00	1233.0
50.00	5104.0
51.00	1834.0
52.10	128.0
54.90	157.0
56.00	441.0
57.10	941.0
60.00	278.0
61.00	1225.0
62.00	1434.0
63.10	1301.0
63.90	293.0
65.10	329.0
67.00	108.0
68.00	2681.0
69.00	2769.0
70.00	301.0
72.00	146.0
73.00	1046.0
74.10	4426.0
75.10	13714.0
76.00	1155.0
77.10	158.0
78.00	110.0
78.90	922.0
79.90	302.0
80.90	956.0
81.90	206.0
86.10	115.0
87.00	1055.0
88.00	925.0
90.80	151.0
92.00	895.0
93.00	1165.0
94.00	3135.0
95.10	25832.0
96.00	1671.0
103.80	122.0
105.90	159.0
115.80	112.0
117.00	237.0
117.80	125.0
118.90	184.0
127.80	162.0
129.90	110.0
140.90	318.0
142.90	445.0
144.90	181.0
154.80	110.0
171.90	246.0
174.00	21680.0
175.00	1585.0
176.00	20688.0
177.00	1368.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	217.0
37.00	1494.0
38.10	1102.0
39.00	597.0
39.90	127.0
44.00	1063.0
45.00	333.0
45.90	116.0
47.00	322.0
47.90	281.0
49.10	1352.0
50.10	5481.0
51.00	1807.0
52.10	137.0
54.90	144.0
56.00	471.0
57.00	954.0
60.00	332.0
61.00	1285.0
62.00	1578.0
63.10	1320.0
63.90	340.0
65.10	334.0
66.90	141.0
68.00	2912.0
69.00	3088.0
69.90	332.0
72.00	180.0
73.00	1121.0
74.00	4593.0
75.10	14304.0
76.00	1147.0
77.10	201.0
78.00	160.0
78.90	1004.0
79.90	310.0
80.90	1142.0
81.90	235.0
87.00	1073.0
88.00	1011.0
90.70	138.0
92.00	954.0
93.00	1220.0
94.00	3302.0
95.10	27592.0
96.00	1686.0
103.80	142.0
105.90	183.0
115.80	120.0
117.00	239.0
117.90	113.0
118.90	199.0
127.80	158.0
129.90	138.0
140.80	316.0
142.90	524.0
144.90	194.0
154.80	138.0
171.90	283.0
174.00	24040.0
175.00	1624.0
176.00	22928.0
177.00	1450.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

m/z	Abundance
36.00	175.0
37.10	1461.0
38.10	1014.0
39.00	533.0
39.90	124.0
44.00	1119.0
45.00	318.0
47.10	290.0
47.90	269.0
49.10	1339.0
50.00	5268.0
51.00	1571.0
52.10	127.0
54.90	122.0
56.00	439.0
57.00	844.0
60.00	324.0
61.00	1201.0
62.00	1477.0
63.00	1188.0
63.90	295.0
65.10	357.0
67.00	172.0
68.00	2951.0
69.00	3056.0
70.00	288.0
72.00	198.0
73.10	1175.0
74.00	4374.0
75.00	13438.0
76.00	1017.0
77.10	225.0
78.90	991.0
79.90	283.0
80.90	1141.0
81.90	253.0
87.00	1098.0
87.90	1043.0
90.80	107.0
92.00	914.0
93.00	1167.0
94.00	3039.0
95.10	26408.0
96.00	1563.0
103.90	156.0
105.90	190.0
115.80	115.0
116.90	207.0
117.90	106.0
118.90	224.0
127.80	130.0
129.90	138.0
140.80	281.0
142.90	573.0
144.90	195.0
154.80	142.0
171.90	300.0
174.00	23392.0
175.00	1567.0
176.00	22904.0
177.00	1445.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83

Scan 2790 (10.061 min): VV019125.D
BFB83

m/z	Abundance
40.10	157.0
44.00	851.0

Instrument :
MSVOA_V
ClientSampleId :
BFB83