


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023064.D
Acq On : 27 Oct 2021 17:34
Operator : SY/MD
Sample : M4278-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 10/29/2021
Supervised By :Semsettin Yesilyurt 11/02/2021

Quant Time: Oct 28 01:47:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 01:43:46 2021
Response via : Initial Calibration

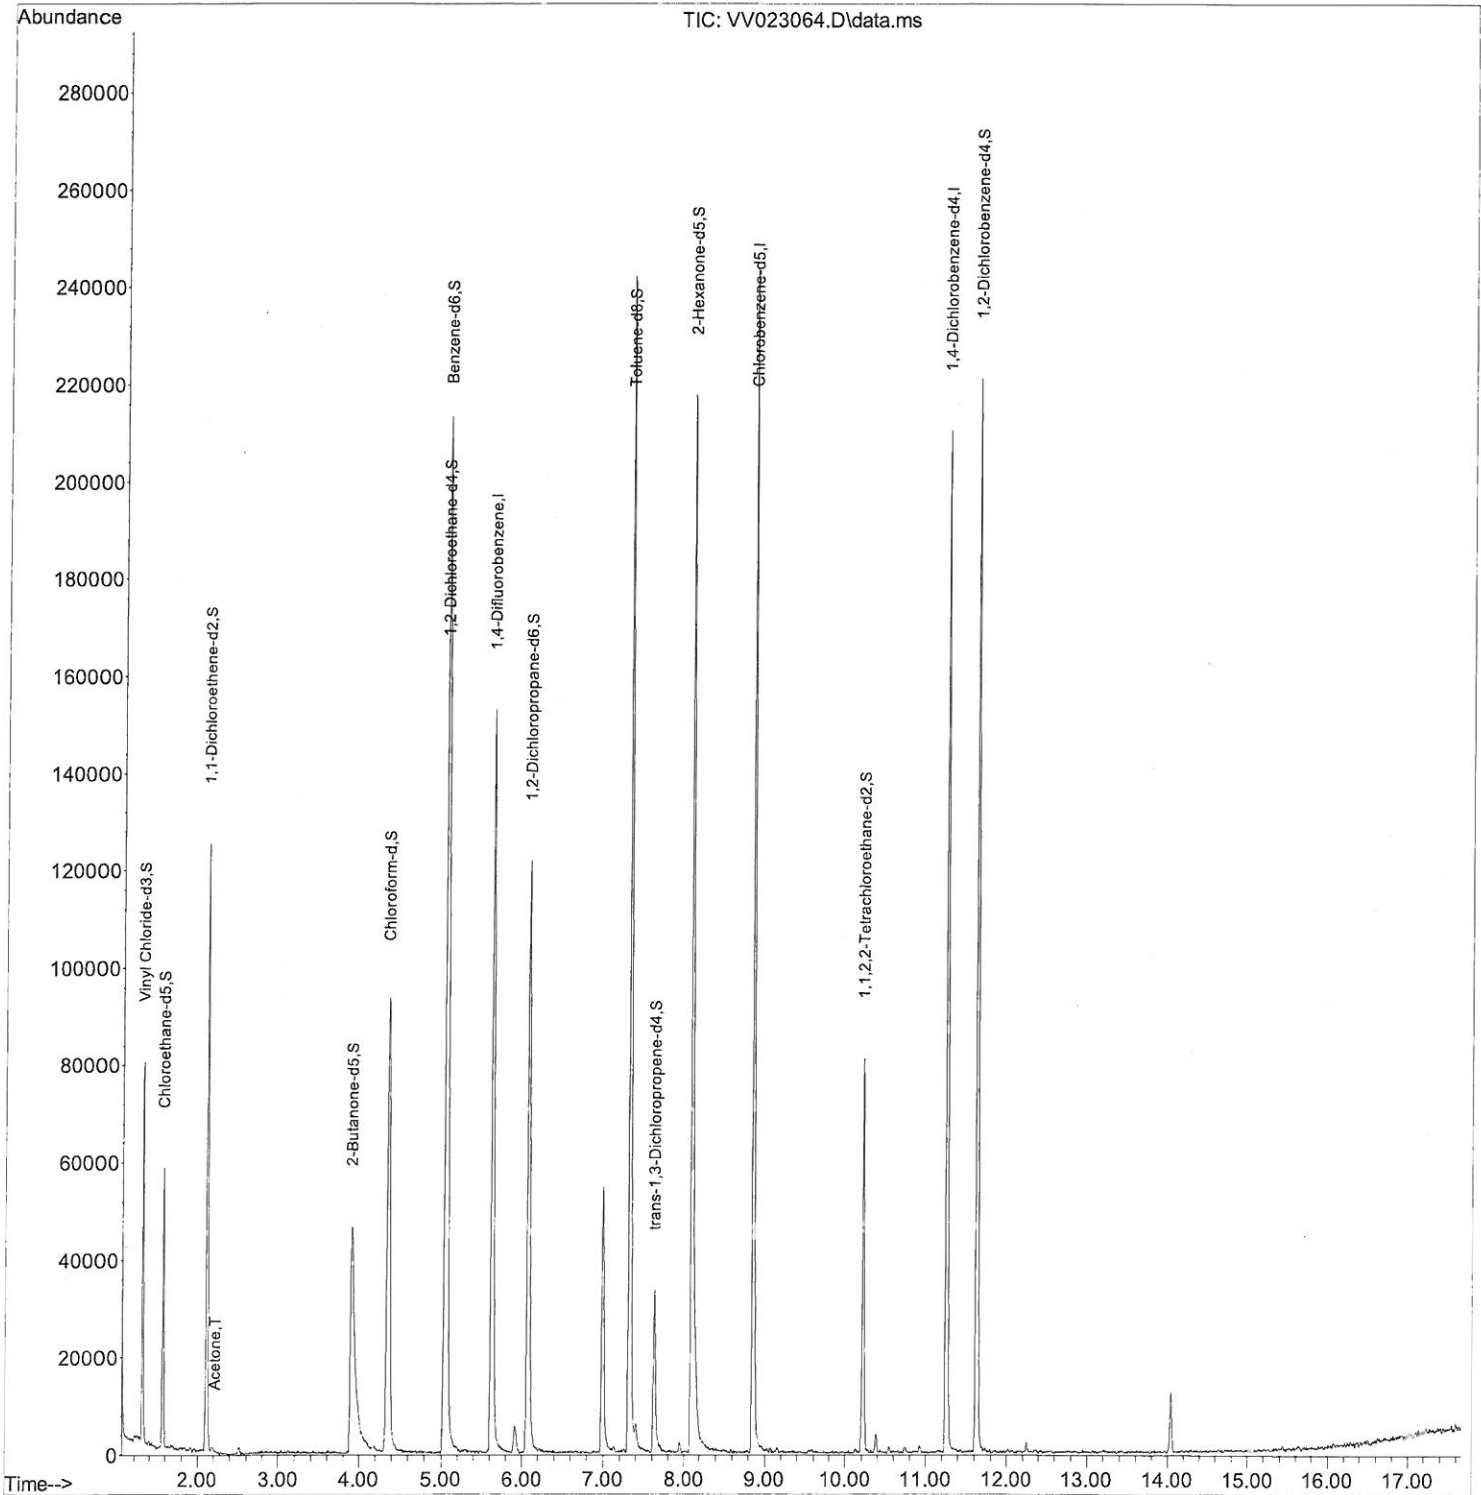

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023064.D
 Acq On : 27 Oct 2021 17:34
 Operator : SY/MD
 Sample : M4278-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Oct 28 01:47:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 01:43:46 2021
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/29/2021
 Supervised By :Semsettin Yesilyurt 11/02/2021

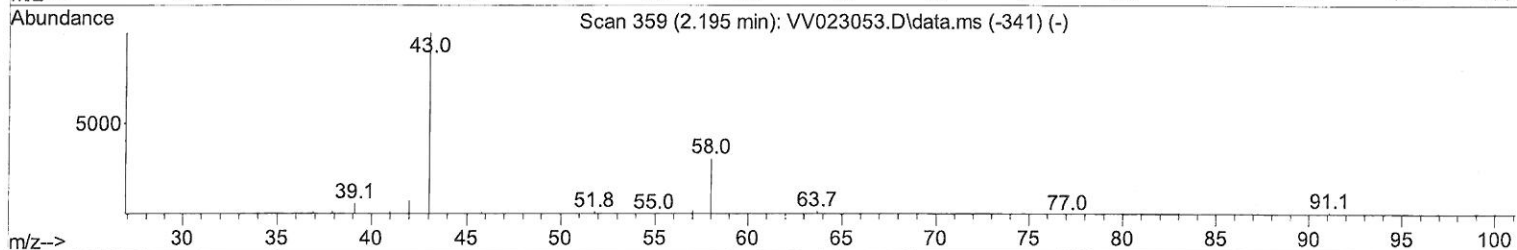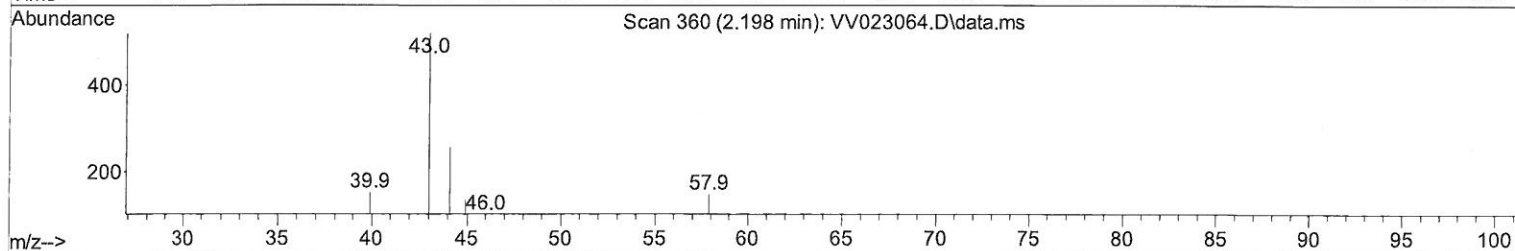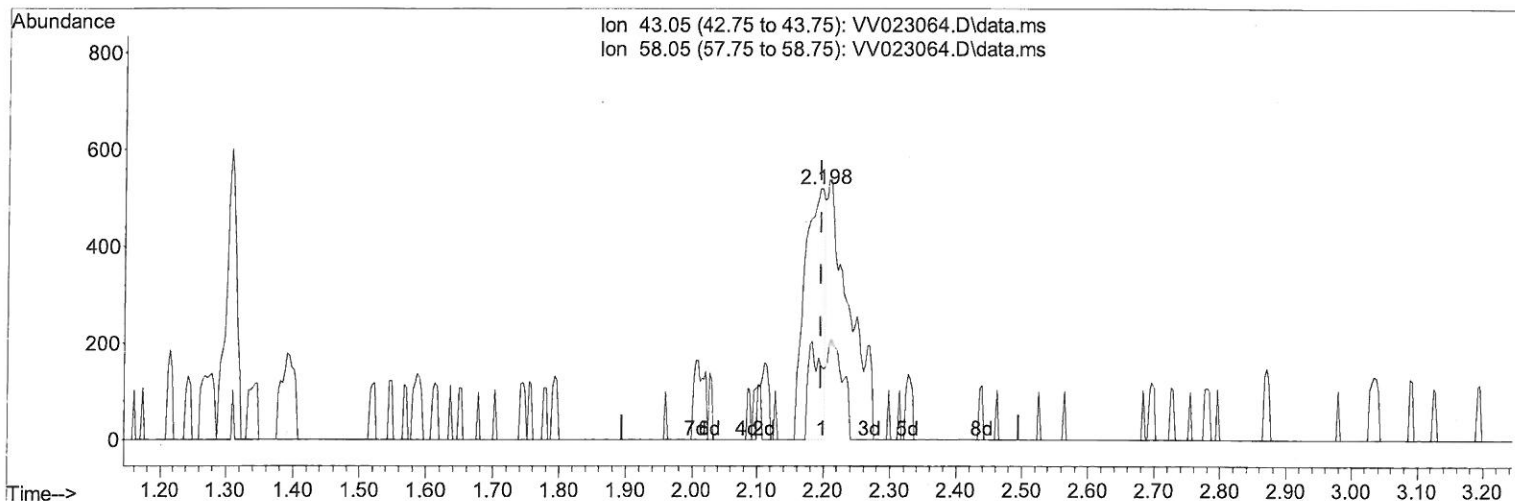

TIC: VV023064.D\data.ms

(13) Acetone (T)

2.198min (+ 0.003) 1.18 ug/L

response 1089

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	31.40
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023064.D
Acq On : 27 Oct 2021 17:34
Operator : SY/MD
Sample : M4278-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Oct 28 01:47:41 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 01:43:46 2021
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 10/29/2021
Supervised By :Semsettin Yesilyurt 11/02/2021

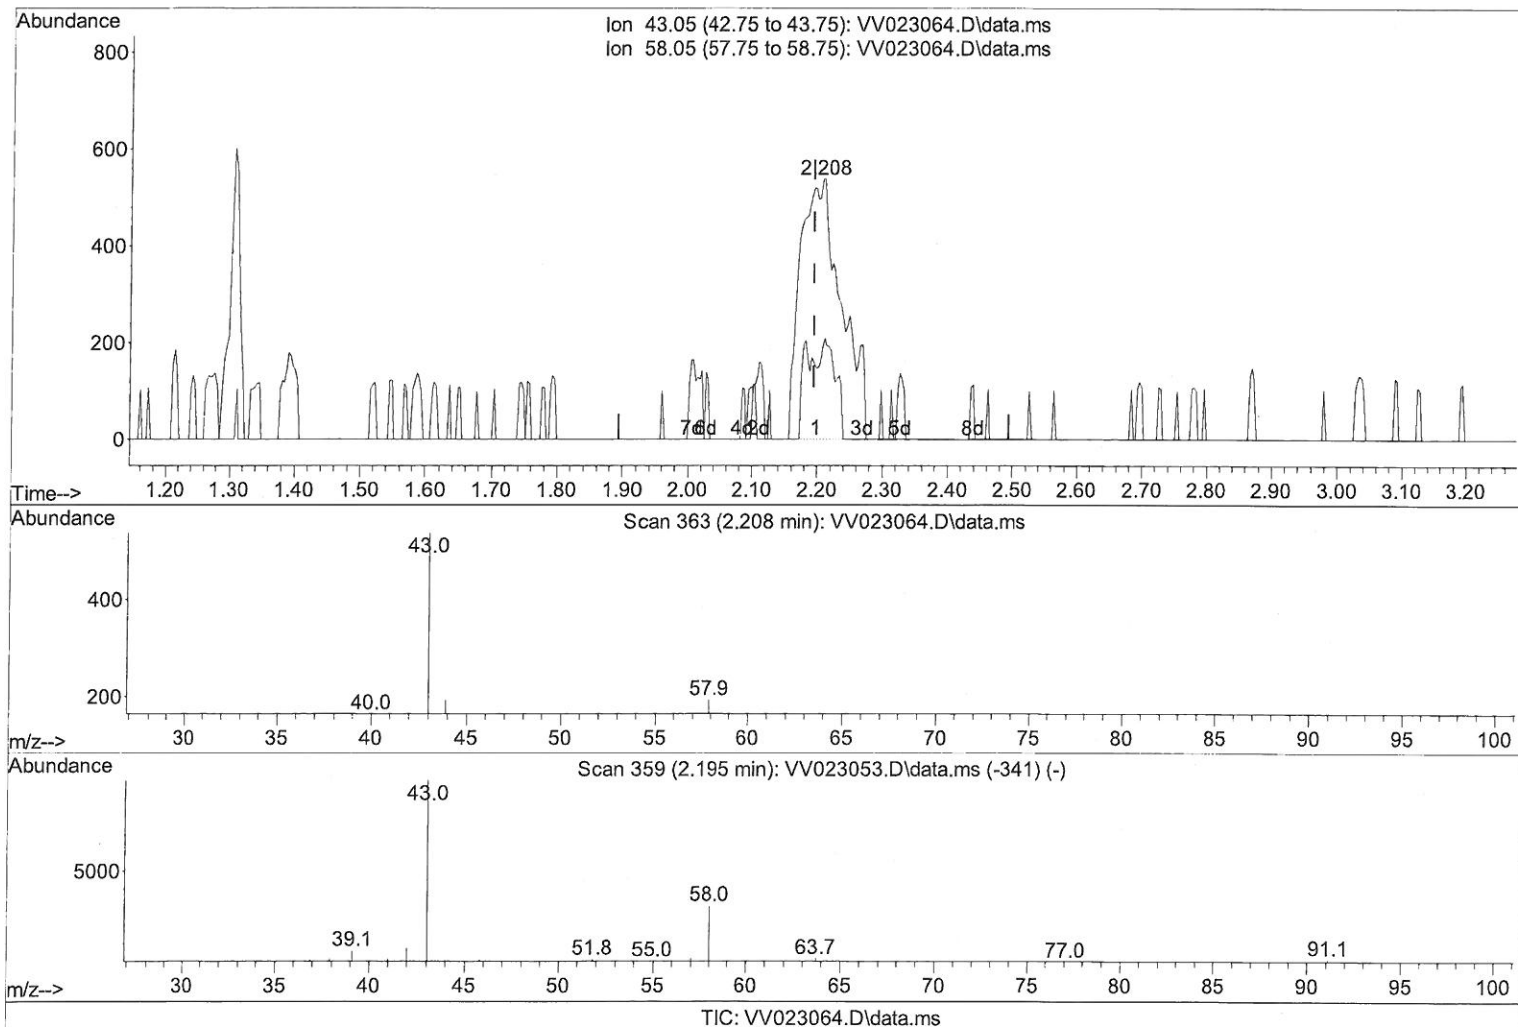

(13) Acetone (T)

2.208min (+ 0.013) 2.55 ug/L m

response 2353

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	14.53
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
11/02/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023064.D
 Acq On : 27 Oct 2021 17:34
 Operator : SY/MD
 Sample : M4278-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual Integrations APPROVED

Reviewed By : Mahesh Dadoda 10/29/2021
 Supervised By : Semsettin Yesilyurt 11/02/2021

Quant Time: Oct 28 01:47:41 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 01:43:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	134126	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	135301	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	57374	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	47909	4.088	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	81.800%	
7) Chloroethane-d5	1.568	69	36109	4.981	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	99.600%	
11) 1,1-Dichloroethene-d2	2.108	63	59321	3.509	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	70.200%	
20) 2-Butanone-d5	3.899	46	112198	59.677	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	119.360%	
24) Chloroform-d	4.349	84	98786	5.185	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	103.600%	
26) 1,2-Dichloroethane-d4	5.037	65	46855	5.217	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	104.400%	
32) Benzene-d6	5.053	84	195646	4.953	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.000%	
36) 1,2-Dichloropropane-d6	6.072	67	63254	5.202	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	104.000%	
41) Toluene-d8	7.317	98	163008	4.594	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.800%	
43) trans-1,3-Dichloroprop...	7.625	79	19945	4.681	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	93.600%	
46) 2-Hexanone-d5	8.092	63	72313	45.843	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	91.680%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	39450	4.698	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	94.000%	
66) 1,2-Dichlorobenzene-d4	11.625	152	60429	5.903	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	118.000%	

Target Compounds

	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	2.208	43	2353m	2.551	ug/L	7 MD

(#) = qualifier out of range (m) = manual integration (+) = signals summed