

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023063.D
 Acq On : 27 Oct 2021 17:10
 Operator : SY/MD
 Sample : M4277-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 28 01:47:25 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 01:43:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	131370	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	134334	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	57608	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46396	4.042	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.800%
7) Chloroethane-d5	1.568	69	32381	4.560	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.200%
11) 1,1-Dichloroethene-d2	2.108	63	44963	2.715	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	54.400%#
20) 2-Butanone-d5	3.886	46	110847	60.195	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	120.400%
24) Chloroform-d	4.352	84	98043	5.254	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	105.000%
26) 1,2-Dichloroethane-d4	5.034	65	45319	5.152	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.000%
32) Benzene-d6	5.053	84	191574	4.885	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	6.072	67	60434	5.006	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	100.200%
41) Toluene-d8	7.320	98	159522	4.528	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.600%
43) trans-1,3-Dichloroprop...	7.625	79	20169	4.768	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.400%
46) 2-Hexanone-d5	8.088	63	72143	46.065	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	92.120%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	38383	4.604	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.000%
66) 1,2-Dichlorobenzene-d4	11.625	152	59982	5.836	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	116.800%
Target Compounds					Qvalue	
13) Acetone	2.179	43	2972	3.290	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023063.D
Acq On : 27 Oct 2021 17:10
Operator : SY/MD
Sample : M4277-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 28 01:47:25 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 01:43:46 2021
Response via : Initial Calibration

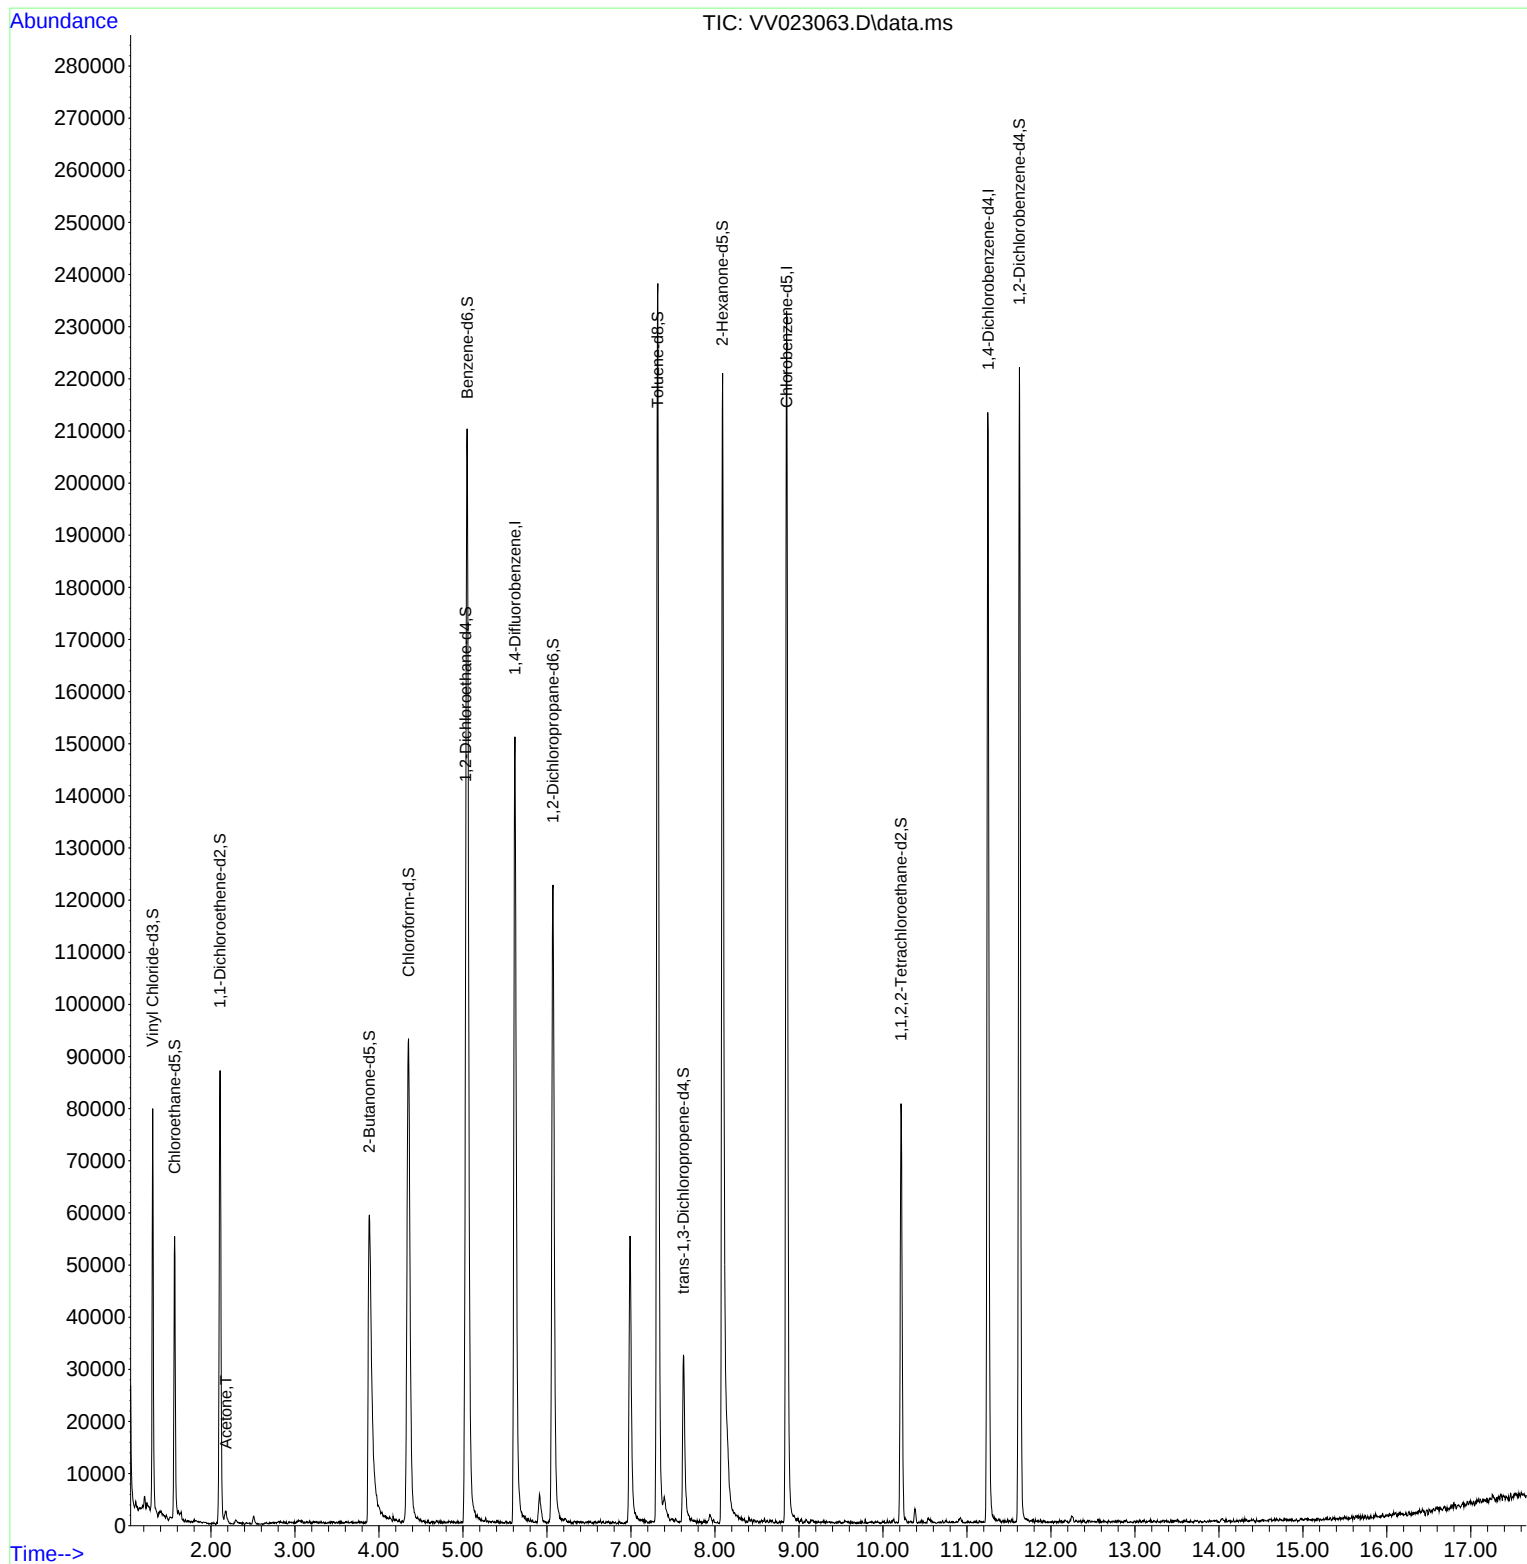

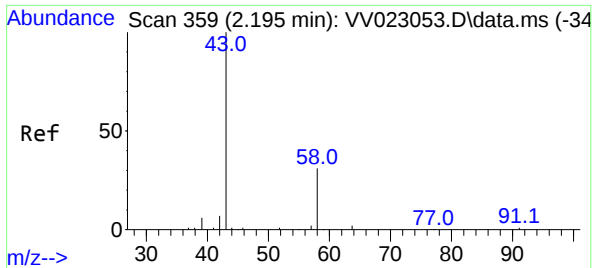

#13
 Acetone
 Concen: 3.290 ug/L
 RT: 2.179 min Scan# 31
 Delta R.T. -0.016 min
 Lab File: VV023063.D
 Acq: 27 Oct 2021 17:10

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 43 Resp: 2972
 Ion Ratio Lower Upper
 43 100
 58 31.3 0.0 55.4

