

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
 Data File : VV023066.D
 Acq On : 27 Oct 2021 18:46
 Operator : SY/MD
 Sample : M4364-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG324

Quant Time: Oct 28 01:48:17 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 01:43:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	130435	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	136292	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	59353	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	46447	4.075	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	81.600%
7) Chloroethane-d5	1.567	69	30516	4.328	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	86.600%
11) 1,1-Dichloroethene-d2	2.108	63	54228	3.298	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	66.000%
20) 2-Butanone-d5	3.886	46	103529	56.624	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	113.240%
24) Chloroform-d	4.349	84	96192	5.191	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	103.800%
26) 1,2-Dichloroethane-d4	5.034	65	45854	5.250	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	105.000%
32) Benzene-d6	5.053	84	188023	4.725	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.600%
36) 1,2-Dichloropropane-d6	6.072	67	60695	4.955	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	99.200%
41) Toluene-d8	7.316	98	161599	4.521	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.400%
43) trans-1,3-Dichloroprop...	7.625	79	17426	4.060	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.200%
46) 2-Hexanone-d5	8.088	63	74551	46.918	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.840%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	40018	4.731	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.600%
66) 1,2-Dichlorobenzene-d4	11.625	152	60804	5.742	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.800%
Target Compounds						
					Qvalue	
13) Acetone	2.175	43	1418	1.581	ug/L	86


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023066.D
Acq On : 27 Oct 2021 18:46
Operator : SY/MD
Sample : M4364-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG324

Quant Time: Oct 28 01:48:17 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 01:43:46 2021
Response via : Initial Calibration

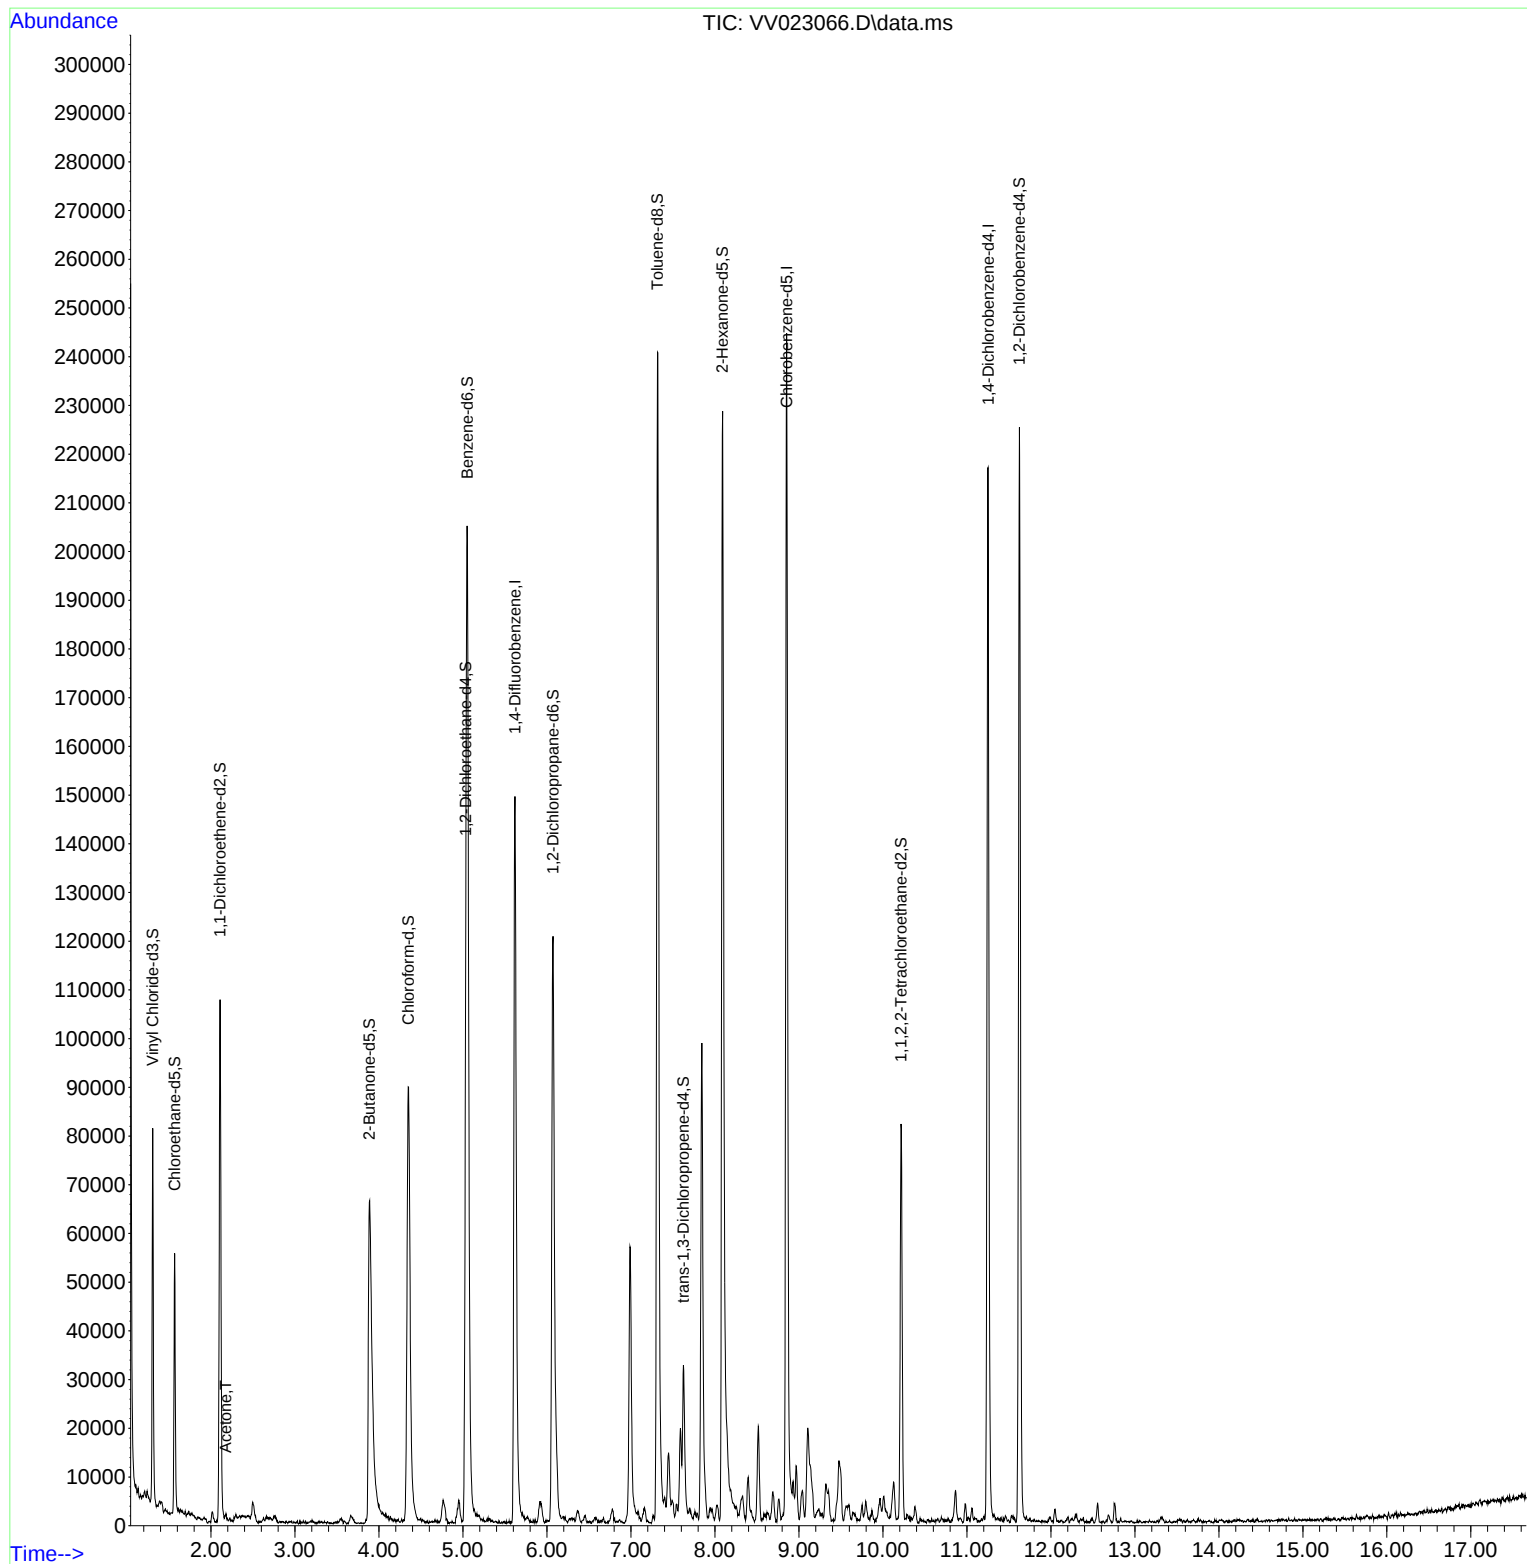

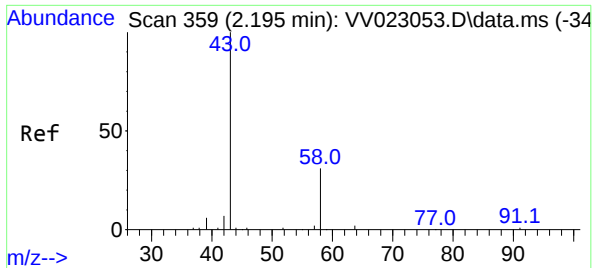

#13
 Acetone
 Concen: 1.581 ug/L
 RT: 2.175 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV023066.D
 Acq: 27 Oct 2021 18:46

Instrument :
 MSVOA_V
 ClientSampleId :
 BG324

Tgt Ion: 43 Resp: 1418
 Ion Ratio Lower Upper
 43 100
 58 20.2 0.0 55.4

