

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW102721\
 Data File : VW023071.D
 Acq On : 27 Oct 2021 20:46
 Operator : SY/MD
 Sample : M4277-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Oct 28 01:49:44 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Oct 28 01:43:46 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	127698	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	134776	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	57660	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	44157	3.957	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	79.200%
7) Chloroethane-d5	1.565	69	24085	3.489	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	69.800%
11) 1,1-Dichloroethene-d2	2.108	63	50406	3.131	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	62.600%
20) 2-Butanone-d5	3.886	46	99495	55.584	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	111.160%
24) Chloroform-d	4.349	84	90727	5.001	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.000%
26) 1,2-Dichloroethane-d4	5.034	65	43010	5.030	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	100.600%
32) Benzene-d6	5.050	84	180199	4.580	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.600%
36) 1,2-Dichloropropane-d6	6.072	67	59727	4.931	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	98.600%
41) Toluene-d8	7.317	98	151439	4.285	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	85.600%
43) trans-1,3-Dichloroprop...	7.625	79	17955	4.231	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.600%
46) 2-Hexanone-d5	8.092	63	68892	43.844	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	87.680%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	37268	4.456	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	89.200%
66) 1,2-Dichlorobenzene-d4	11.625	152	56660	5.507	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.200%
Target Compounds					Qvalue	
13) Acetone	2.176	43	1518	1.729	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV102721\
Data File : VV023071.D
Acq On : 27 Oct 2021 20:46
Operator : SY/MD
Sample : M4277-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Oct 28 01:49:44 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR102221WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Oct 28 01:43:46 2021
Response via : Initial Calibration

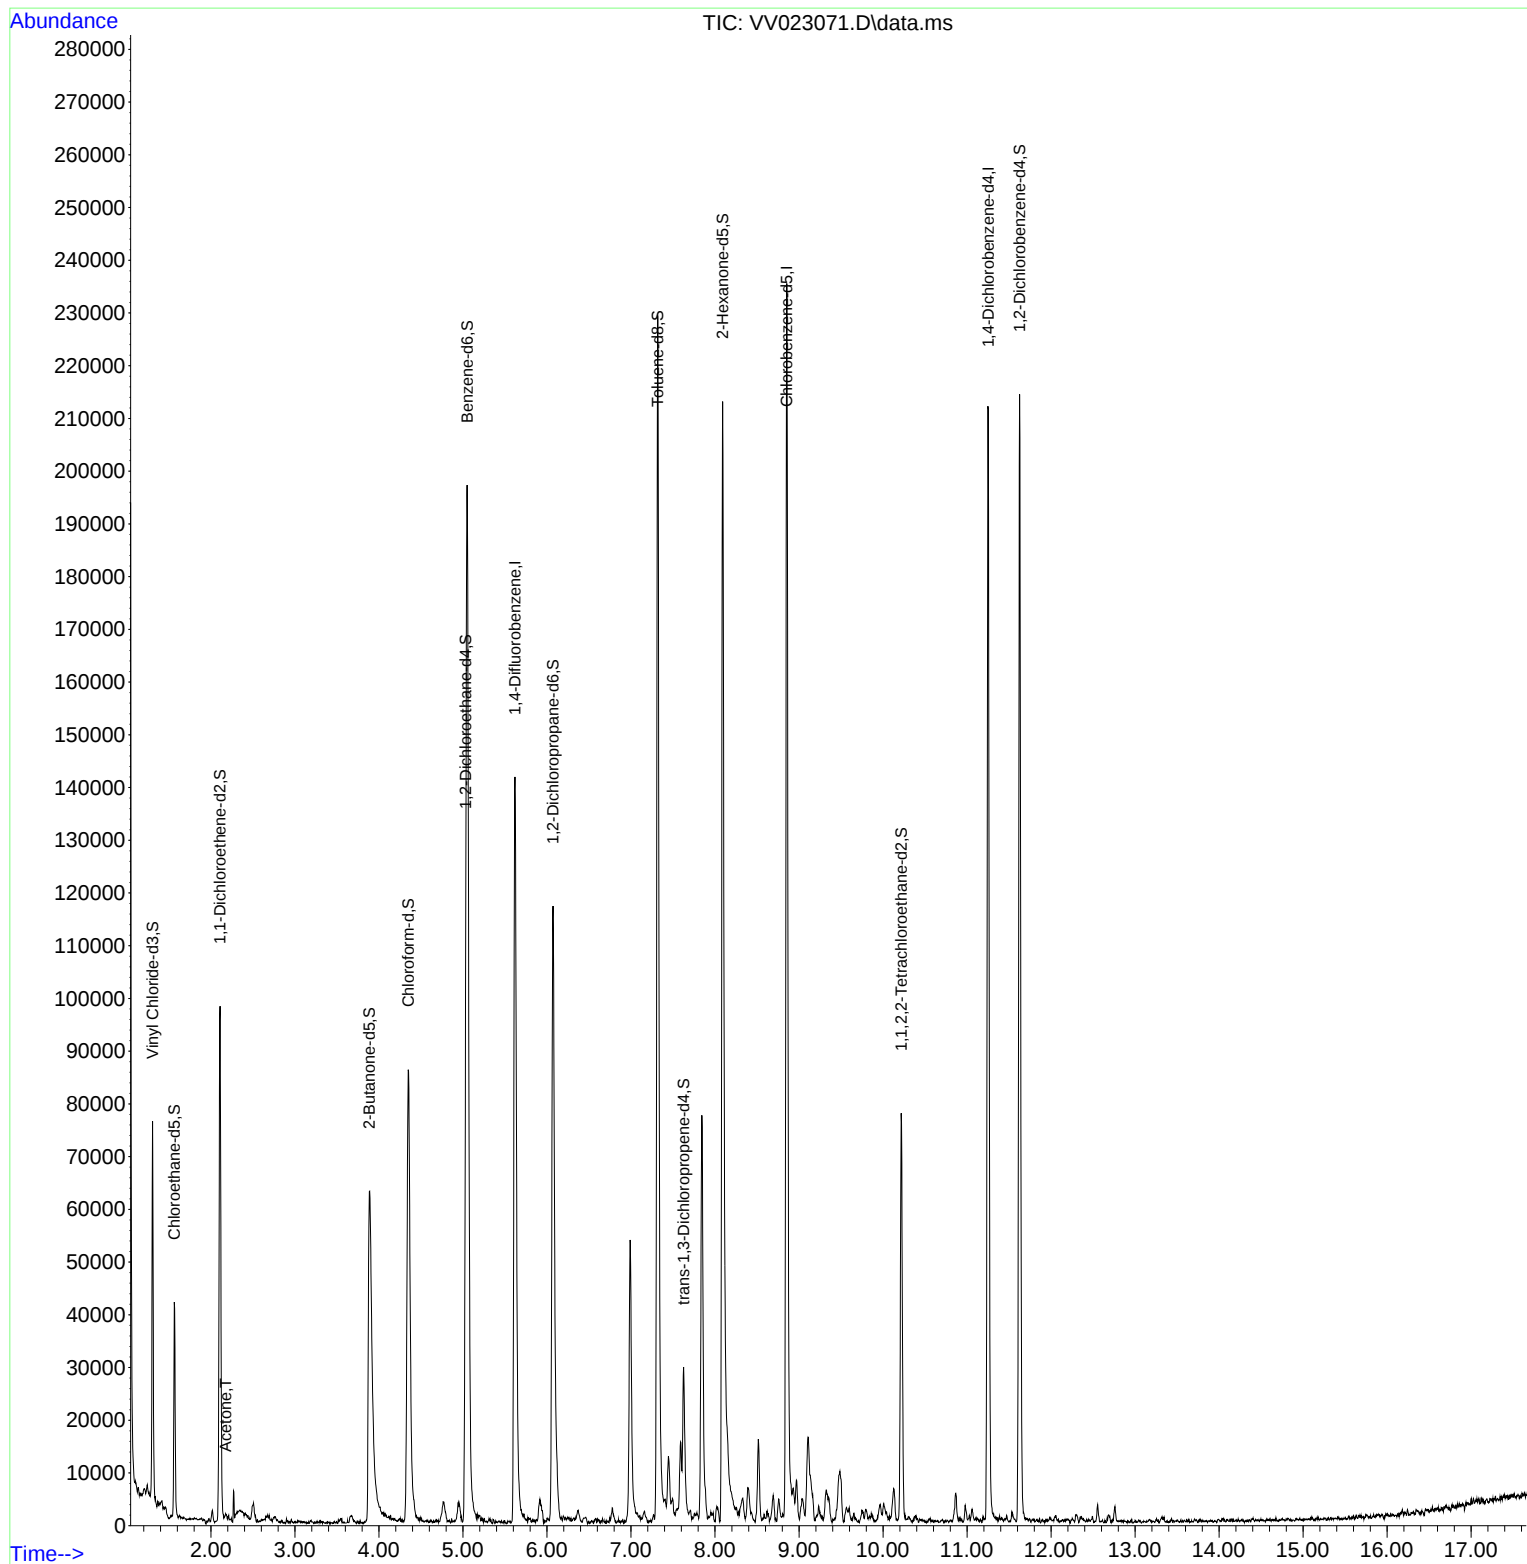

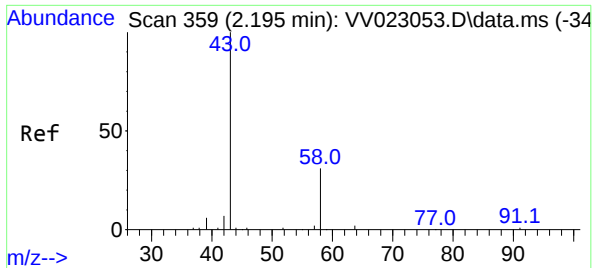

#13
 Acetone
 Concen: 1.729 ug/L
 RT: 2.176 min Scan# 31
 Delta R.T. -0.019 min
 Lab File: VV023071.D
 Acq: 27 Oct 2021 20:46

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Tgt Ion: 43 Resp: 1518
 Ion Ratio Lower Upper
 43 100
 58 27.6 0.0 55.4

